

# User Manual

**EMCPro<sup>TM</sup>**

Advanced EMC Immunity Test System





# EMCPro

## Advanced EMC Immunity Test System

The EMCPro is an advanced EMC immunity test system developed by KeyTek in response to manufacturers' demands for a mid-range, low cost, multi-capability test system. The EMCPro is easily configured to meet today's immunity standards required for CE Marking and compliance requirements. In addition, EMCPro capabilities go well beyond the required test levels for the CE Mark.

The EMCPro performs compliance level testing requirements for IEC, UL, ANSI, ETSI and beyond. The EMCPro allows users to perform compliance testing to the following standards:

EN 50082-1	IEC 1000-4-8	Power Frequency Magnetic Fields
EN-50082-2		
CCITT K17, K20, K21	IEC 1000-4-9	Pulse Magnetic Fields
ETSI	IEC 1000-4-11	Dips and Interrupts
UL 1449	IEC 1000-4-12	100kHz Ring Wave
IEC 1000-4-2 ESD	UL 864	
IEC 1000-4-4 EFT	ANSI/IEEE C62.41	
IEC 1000-4-5 Combination and Telecom Wave Surge		

Users may operate the EMCPro via KeyTek's easy to use Windows-based PC software, *CEWare*, or from the front panel. *CEWare* provides simple, straight forward pre-programmed test sequences ideal for the novice user; yet is sophisticated enough to allow an advanced user to develop and save custom test sequences for future testing.

Users may configure the EMCPro from a single test capability to up to seven capabilities in a single unit. When test requirements change, or as standards evolve, upgrading is a simple matter of adding appropriate options or accessories offered by KeyTek to their existing EMCPro.

One System, One Vendor, One Solution.

The EMCPro system offers the highest test levels and the widest selection of testing capabilities in a low-cost complete system solution.





KeyTek  
One Lowell Research Center  
Lowell, MA 01852-4345  
TEL: (978) 275-0800  
FAX: (978) 275-0850  
<http://www.keytek.com>

## ***SPECIAL NOTES FOR THE EMCPro***

The *EMCPro* has incorporated a special, relay-cleaning sequence. Before any surge operation – 1.2/50, 10/700, Ringwave, or Pulsed Magnetic Field (PMF) – the relays within the *EMCPro* are cycled rapidly, usually in a sequence of five and five clicks or five and three.

This is normal behavior and not a cause for concern.

The relay-cleaning sequence removes oxidation and pitting from the surface of the relay contacts, for better operation and longer relay life.



# EMC Pro<sup>TM</sup>

## Advanced EMC Immunity Test System

### TECHNICAL SPECIFICATIONS

#### MODEL PRO-ESD

*ESD per IEC 1000-4-2*

Trigger Modes:	One shot manual, multi-shot tripod
Repetition Rate:	Single shot, 1pps or 20pps
Air Discharge Voltage:	500V - 8.8kV $\pm 10\%$
Contact Discharge Voltage:	500V - 4.4kV $\pm 10\%$
Discharge Capacitor:	150pF $\pm 10\%$
Discharge Resistance:	330 $\Omega$ $\pm 10\%$
Charging Resistance:	50M $\Omega$ - 100M $\Omega$
Polarity:	Front panel or software controlled
Shot Counter:	1 - 999 discharges
Energy Storage:	5.8mJ @ 8.8kV

#### MODEL PRO-EFT

*EFT per IEC 1000-4-4 and ANSI*

Voltage Waveform:	5/50ns $\pm 30\%$
Peak Voltage:	250V - 4.4kV $\pm 5\%$
Burst Period:	300ms $\pm 10\%$
Burst Duration:	15ms $\pm 20\%$
Frequency:	1-100kHz, in 0.5kHz steps, $\pm 10\%$
DC Blocking Capacitor:	10nF (internal)

#### MODEL PRO-SURGE

*Surge per IEC 1000-4-5, ANSI and UL*

Voltage Waveform:	1.2/50 $\mu$ s
Peak Voltage:	250V - 6.6kV $\pm 5\%$ , 12 $\Omega$ mode 250V - 6.0kV $\pm 5\%$ , 2 $\Omega$ mode
Peak Current:	125A - 3.3kA $\pm 10\%$
Additional 10 $\Omega$ Resistor:	Software selectable
Repetition Rate:	up to 4 per minute
Open-circuit Voltage:	Front time: 1.2 $\mu$ s $\pm 30\%$ Duration: 50 $\mu$ s $\pm 20\%*$ Undershoot: $\leq 30\%$
Short-circuit Current:	Front time: 8.0 $\mu$ s $\pm 20\%$ Duration: 20 $\mu$ s $\pm 20\%$ Undershoot: $\leq 30\%$
Line sync accuracy:	$\pm 15\%$ , 50 - 277VAC

\* Durations are reduced in 12 $\Omega$  mode and with multiple lines to PE coupling modes.

#### MODEL PRO-RING\*

*Surge Ring Wave per ANSI and UL*

Voltage Waveform:	100kHz damped cosine
Peak Voltage:	250 - 6.6kV $\pm 5\%$
Repetition Rate:	up to 6 per minute
Open-circuit Voltage:	Rise Time: 0.5 $\mu$ s $\pm 30\%$
Short-circuit Current:	Vp/Ip: 12 $\Omega$ $\pm 3\Omega$ or 30 $\Omega$ $\pm 8\Omega$ software selectable



#### MODEL PRO-TELECOM\*

*Surge Telecom per IEC 1000-4-5, FCC, CCITT and ETSI*

Voltage Waveform:	10/700 $\mu$ s (9/720 $\mu$ s FCC Part 68)
Peak Voltage:	250V - 6.6kV $\pm 5\%$
Peak Current:	6.25 - 165A $\pm 10\%$ , 40 $\Omega$ mode
Repetition Rate:	up to 4 per minute
Open-circuit Voltage:	Front time: 7.0 $\mu$ s to 11.7 $\mu$ s Duration: 576 $\mu$ s to 840 $\mu$ s
Short-circuit Current:	Front time: 3.5 $\mu$ s to 6.5 $\mu$ s Duration: 256 $\mu$ s to 384 $\mu$ s

#### SURGE WAVEFORM MONITORING

Lines Monitored:	Monitors are automatically switched to match generator coupling mode
Open-circuit Voltage:	1000:1 $\pm 10\%$
Short-circuit Current Attenuation:	200:1 $\pm 7\%$

#### MODEL PRO-HPOWER

*Power Frequency Magnetic Field per IEC 1000-4-8*

Field Frequency:	50Hz/60Hz
Field Amplitude:	0.5 - 4A/m, in 0.25A steps, $\pm 10\%$ (with CM-HCOIL) up to 100A/m with optional external HPOWER-EXT
AC Source:	Internal
Resolution:	0.25A minimum
Coil Factor:	0.65 to 1.00
Coil Resistance:	0.05 $\Omega$ maximum

## TECHNICAL SPECIFICATIONS

### MODEL PRO-HPULSE

*Pulse Magnetic Field per IEC 1000-4-9*

Field Pulse:	8/20 $\mu$ s
Field Amplitude:	100A/m - 1000A/m, $\pm$ 10%
Resolution:	5A/m
Coil Factor:	0.65 to 1.00

### MODEL PRO-PQF

*Dips and Interrupts per IEC 1000-4-11*

Dips:	70%, 40%
Interrupts:	0% (short and open)
Transition Time:	1 $\mu$ s - 5 $\mu$ s
Inrush:	Minimum 250Amps @ 100 - 120V, Minimum 500Amps @ 220 - 240V
AC Voltage:	50 - 250VAC, 50/60Hz
AC Current:	16A max.**
PQF Sync Output:	5V signal occurs at each dip or interrupt transition

### PQF WAVEFORM MONITORING

Voltage Input Connection:	Fixed, L1 to L2
Voltage Attenuation:	100:1 $\pm$ 5%
Current Input Connection:	Fixed, L1
Peak Current:	Minimum 500A inrush into 1700 $\mu$ F
Current Attenuation:	200:1 $\pm$ 5%

## MODEL PRO-BASE

**SYSTEM VOLTAGE** 90-240VAC, 50/60Hz

**INTEGRATED EUT MAINS COUPLER/DECOUPLER**

AC Voltage:	1 phase, 50 - 250VAC, 50/60Hz
AC Current:	16A max.**
DC Voltage:	100VDC max.
DC Current:	10A max.
Frequency:	50/60Hz

**EUT Connectors:** Nema, British, Schuko

**CONTROL INTERFACE**

**Interface:** RS232 Fiber-optic

**SAFETY FEATURES**

- External Interlock for users
- Interlock for CCL connector
- External stop input

**ENVIRONMENTAL OPERATING CONDITIONS**

Temperature:	15- 40°C
Humidity:	10-75%, non-condensing
Altitude:	8000 ft. max.

**PHYSICAL**

Height:	22.9cm (8.7 in)
Width:	43.4cm (17.1 in)
Depth:	64.8cm (25.5 in)
Weight:	39kg (85 lbs)

## OPTIONAL COUPLER/DECOUPLERS

### MODEL CM-3CD-16 & CM-3CD-32

*Semi-automatic, stand alone, three-phase EFT & Surge AC/DC mains coupler/decouplers*

AC Voltage:	0 to 250/433VAC, 50/60Hz **
AC Current CM-3CD-16:	16A/phase continuous
AC Current CM-3CD-32:	32A/phase continuous
DC Voltage:	100VDC max.
DC Current:	10A max.
EUT Connectors:	Safety Sockets

### MODEL CM-3PQF

*Semi-automatic, 3-phase Dip/Interrupt Selector*

AC Voltage:	50 to 250/433VAC, 50/60Hz **
AC Current:	16A/phase continuous **
EUT Connectors:	Safety Sockets

### MODEL CM-I/OCD

*External, 8-line coupler/decoupler for signal lines*

Waveforms:	Couples combination waves of 1.2/50 $\mu$ s open-circuit voltage, 8/20 $\mu$ s short-circuit current
Data Line Freq:	> 100kHz with HS option
Number of Lines:	Eight lines
Surge Voltage:	4.4kV max.
Signal Line Voltage:	200V peak max.
Signal Line Current:	1A max.
Clamping:	Selectable built-in clamps of 20V and 220V: external bias input for other clamp levels

### MODEL CM-TELCD

*External coupler/decoupler for Telecom lines*

Waveforms:	Couples 1.2/50 $\mu$ s Combination and 10/700 $\mu$ s Telecom waves
Data Line Freq:	To 100kHz without degradation
Number of Lines:	Up to four lines - one or two pairs of balanced Telecom lines.
Surge Voltage:	4.4kV max.
Signal Line Voltage:	200V peak max.
Signal Line Current:	1A max.
Clamping:	Selectable built-in clamps of 20V and 220V: external bias input for other clamp levels

\* Pro-Telecom and Pro-Ring can not be installed together in the same unit.

\*\* The actual AC mains current and voltage rating is based on the mains connector selected.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company

KeyTek is a registered trademark and EMCPro is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.

KPS-749B-9/98



---

# TABLE OF CONTENTS

## OVERVIEW

PRODUCT SAFETY INFORMATION .....	IV
PRODUCT SAFETY .....	1
SURGE TESTING GUIDELINES .....	3
SAFETY CONCERNS DURING SURGE TESTING .....	4
INAPPROPRIATE USES .....	5
DESCRIPTION.....	6
INSTALLATION.....	7
UNPACKING INSTRUCTIONS .....	7
HANDLING, TRANSPORTATION, STORAGE.....	7
CABLING AND INTERCONNECTIONS .....	8
ELECTRICAL SUPPLY REQUIREMENTS.....	12
PHYSICAL ENVIRONMENT.....	14
OPERATING LIMITS.....	14
STORAGE LIMITS .....	14
TEST AREA CONSIDERATIONS AND SITE PREPARATION .....	15
SPECIAL CONSIDERATIONS FOR SURGE TESTING.....	15
SPECIAL CONSIDERATIONS FOR EFT TESTING .....	16
SPECIAL CONSIDERATIONS FOR ESD TESTING.....	19
SPECIAL CONSIDERATIONS FOR PULSED MAGNETIC FIELD AND POWER-FREQUENCY MAGNETIC FIELD TESTING ...	19

## OPERATION

INTRODUCTION .....	21
EMCPro SYSTEM INTERCONNECTIONS -- ESD AND COMPUTER INTERFACE.....	21
USER INTERFACE.....	27
PROGRAMMING THE EMCPro FROM THE FRONT PANEL.....	28
Main Menu.....	28
Test Menu.....	28
Parameter Definition Menu .....	29
Run Menu.....	30
MAP OF FRONT PANEL MENU STRUCTURE .....	34
PROGRAMMING THE EMCPro FROM A PERSONAL COMPUTER.....	36
RUNNING TESTS.....	38
STANDARDS OVERVIEW .....	38
TEST REQUIREMENTS .....	39
WRITING A TEST PROCEDURE AND THE TEST REPORT .....	39
IEC 1000-4-2 -- ESD TESTING.....	41
What is Electrostatic Discharge (ESD) Testing?.....	41
General Guidelines for ESD Testing .....	42
ESD Testing Requirements per IEC 1000-4-2 .....	43



<i>User-defined ESD Tests</i> .....	45
<i>Preprogrammed IEC Standard ESD Test Sequences</i> .....	45
<i>ESD Waveform Verification</i> .....	46
IEC 1000-4-4 -- EFT TESTING.....	47
<i>What is Electrical Fast Transients (Burst) Testing?</i> .....	47
<i>General Guidelines for EFT Testing</i> .....	48
<i>EFT Testing Requirements per IEC 1000-4-4</i> .....	48
<i>User Defined EFT Test</i> .....	51
<i>Preprogrammed EFT Test Sequences</i> .....	51
<i>EFT Waveform Verification</i> .....	52
SURGE TESTING.....	53
<i>What is Surge Testing?</i> .....	53
<i>General Guidelines for Surge Testing</i> .....	55
<i>Surge Testing Requirements per IEC 1000-4-5</i> .....	58
<i>User Defined Surge Tests</i> .....	60
<i>Preprogrammed IEC Standard Surge Test Sequences</i> .....	62
<i>Surge Waveform Verification</i> .....	65
IEC 1000-4-8 .....	66
POWER-FREQUENCY MAGNETIC FIELD TESTING.....	66
<i>What is Power Frequency Magnetic Field (PFMF) Testing?</i> .....	66
<i>General Guidelines for PFMF Testing</i> .....	66
<i>PFMF Testing Requirements per IEC 1000-4-8</i> .....	67
<i>User Defined Power Frequency Magnetic Field Test</i> .....	68
<i>Preprogrammed IEC Standard PFMF Immunity Test Sequences</i> .....	68
<i>PFMF Waveform Verification</i> .....	68
IEC 1000-4-9 .....	69
PULSED MAGNETIC FIELD TESTING.....	69
<i>What is PULSED MAGNETIC FIELD (PMF) Testing?</i> .....	69
<i>General Guidelines for PMF Testing</i> .....	69
<i>PMF Testing Requirements per IEC 1000-4-9</i> .....	70
<i>PMF User Defined Pulsed Magnetic Field Immunity Test</i> .....	71
<i>Preprogrammed IEC Standard Pulsed Magnetic Field Immunity Test Sequences</i> .....	71
<i>PMF Waveform Verification</i> .....	72
IEC 1000-4-11 .....	73
POWER QUALITY FAILURE TESTING .....	73
<i>What is Power Quality Failure (PQF) Testing?</i> .....	73
<i>General Guidelines for PQF Testing</i> .....	73
<i>Testing Requirements per IEC 1000-4-11</i> .....	74
<i>User Defined PQF Test</i> .....	74
<i>Preprogrammed IEC Standard PQF Test Sequences</i> .....	75
<i>Other Preprogrammed Test Sequences -- Line Qualification</i> .....	76
<i>PQF Waveform Verification</i> .....	77



---

# CEWARE

<b>OVERVIEW OF THE SOFTWARE</b> .....	<b>79</b>
<b>BASIC OPERATIONS</b> .....	<b>80</b>
STARTING THE PROGRAM .....	80
DEFINING A TEST .....	80
RUNNING A TEST .....	80
ADDITIONAL OPERATING NOTES.....	81
CEMASTER/EMCPro DIFFERENCES .....	82
CHANGING PROGRAM SETTINGS .....	83
<b>SCREENS AND ORGANIZATION</b> .....	<b>84</b>
MAIN SCREEN.....	85
NEW SEQUENCE DEFINITION SCREEN .....	89
NEW CUSTOM SEQUENCE WIZARD SCREEN .....	90
SEQUENCE EDITOR SCREEN.....	91
THE RUN SCREEN.....	96
<b>MENU, TOOLBAR, AND STATUS BAR</b> .....	<b>98</b>
MENUBAR.....	98
TOOLBAR.....	106
STATUS BAR .....	106
<i>System Status Bar</i> .....	<i>106</i>

## MAINTENANCE AND TROUBLESHOOTING

<b>MAINTENANCE</b> .....	<b>109</b>
SERVICE AND MAINTENANCE ISSUES.....	109
ANNUAL CALIBRATION .....	109
FACTORY INSPECTION AND REFURBISHMENT .....	109
UPDATING FIRMWARE .....	109
UPGRADING HARDWARE OPTIONS .....	109
DECOMMISSION ISSUES.....	109
<b>TROUBLESHOOTING</b> .....	<b>110</b>
SYSTEM MENU .....	110
TROUBLESHOOTING GUIDE.....	112
ERROR MESSAGES .....	113
<i>Filing a Problem Report</i> .....	<i>115</i>

## DATA SHEETS

## APPLICATION NOTES

---

The information on IEC requirements -- figures and diagrams, tables and data, and test levels -- are accurate as of the date of printing of this manual. However, the IEC and EN documents are subject to review and change. The information in this manual is intended as a guideline only.

---



---

# Product Safety Information

## Definition of Safety-related materials



The lightning flash with arrowhead symbol within an equilateral triangle is intended to alert the user of the presence of uninsulated *dangerous voltages* within the product enclosures, and of voltages upon output connectors, that may be of sufficient magnitude to constitute a risk of electric shock to persons.



The exclamation mark within an equilateral triangle is intended to alert the user of the presence of important operating and maintenance (servicing) instructions in the literature accompanying the product.

## Cautions and Warnings

**-CAUTION-**  
**RISK OF ELECTRIC SHOCK**  
**DO NOT OPEN**

TO REDUCE THE RISK OF SHOCK, DO NOT REMOVE COVER  
NO USER SERVICEABLE PARTS INSIDE  
REFER SERVICING TO QUALIFIED SERVICE PERSONNEL

**WARNING**  
TO PREVENT FIRE OR SHOCK HAZARD,  
DO NOT EXPOSE THIS EQUIPMENT TO RAIN OR MOISTURE





---

# Product Safety

The following safety instructions have been included in compliance with safety standard regulations. Please read them carefully.

- **Read Instructions** -- Read all safety and operating instructions before operating the instrument.
- **Retain Instructions** -- Retain all safety and operating instructions for future reference.
- **Heed Warnings** -- Adhere to all warnings on the instrument and in the operating instructions.
- **Follow Instructions** -- Follow all operating and use instructions.
- **Water and Moisture** -- Do not use the instrument near water.
- **Carts and Stands** -- Use the instrument only with a cart or stand that is recommended or included as part of the **EMCPro** system by the manufacturer.
- **Wall or Ceiling Mounting** -- Do not mount the instrument on a wall or ceiling.
- **Ventilation** -- The instrument should be situated so that its location or position does not interfere with its proper ventilation. Do not install in a cabinet or in other situations that may impede the flow of air through the ventilation openings.
- **Heat** -- The instrument should be situated away from heat sources such as heat registers or other instruments which produce heat.
- **Power Sources** -- Connect the instrument only to the type of power source described in the operating instructions or as marked on the instrument.
- **Grounding or Polarization** -- Take precautions to insure that the grounding of the instrument is not defeated. Operate only with a grounded power cord.
- **Power Cord Protection** -- Place power supply cords so that they are not likely to be walked on or pinched by items placed on them or against them. Pay particular attention to cords at plugs, convenience receptacles, and the point where they enter and exit the instrument. The cordsets used should be the right-angle cordsets supplied with the unit, to prevent damage to the cordsets when moving the **EMCPro**.
- **Cleaning** -- Clean the instrument only as recommended by the manufacturer.

- 
- **Non-Use Periods** -- Unplug the power cords of the instrument when it will be left unused for a long period of time.
  - **Lifting and Carrying** -- When moving or installing an **EMCPro** follow the instructions given in the Installation section of this manual. Moving an **EMCPro** requires two persons.
  - **Object and Liquid Entry** -- Take care that objects do not fall and that liquids are not spilled into the enclosure through openings.
  - **Defects and Abnormal Stress** -- Whenever it is likely that the normal operation has been impaired, make the equipment inoperable and secure it against further operation. Normal operation is likely to be impaired if, for example, the instrument:
    - Shows visible damage.
    - Fails to perform the intended function.
    - Has been subject to prolonged storage under unfavorable conditions.
    - Has been subjected to severe transport stresses.
  - **Damage Requiring Service** -- The instrument should be serviced by qualified service personnel when:
    - The power supply cord or the plug has been damaged.
    - Objects have fallen or liquid has been spilled into the instrument.
    - The instrument has been exposed to rain.
    - The instrument does not appear to operate normally or exhibits a marked change in performance.
    - The instrument has been dropped, or the enclosure has been damaged.
  - **Sitting or Climbing** -- Do not sit or climb upon the instrument or use it as a step or ladder.

---

# Surge Testing Guidelines

- **DO NOT WORK ALONE.**
- Do not use the equipment in conditions other than reasonable laboratory conditions. There should be no condensing humidity or water standing on the floor or work surfaces; there should not be significant dust or other contamination.
- Ensure that **NO ONE** is touching the equipment under test (EUT) during the test or immediately after the test until AC power to the EUT has been turned off.
- Ensure that there is a **barrier** to act as protection in case the equipment under test explodes. This may happen due to power-follow<sup>1</sup> after a failure. The barrier should be interlocked to prevent surging and to disconnect all AC if the barrier is removed.
- The equipment under test must be surrounded by sufficient **insulating material** to withstand twice the surge voltage. Consider distance to the floor or table and walls if air is the insulating material.
- Ensure that the **proper supply mains** voltages are applied to both KeyTek<sup>®</sup> equipment and to the equipment under test, and that the AC branch circuit is capable of supplying the current.
- The ground (protective earth), neutral and phase lines of the AC supply to the equipment under test supply must be connected properly. **Do not defeat the protective earth connection.**
- The ground (protective earth), neutral and phase lines of the AC supply to the KeyTek equipment must be connected properly. **Do not defeat the protective earth connection.**
- When surging a powered EUT, the mains supply to the equipment under test must be capable of handling the potential AC fault current (e.g. do not use a UPS to power the EUT).
- Never surge an AC mains line other than through the EUT output connector and the **EMCPro** internal filter or via a CM-3CD, three-phase coupler.
- Use only equipment which is designed to be safe for the test being performed.
- Do not test in a potentially explosive atmosphere (e.g. where there are gas fumes).
- Never use equipment that is operating in a strange manner, or that shows clear indication of abuse.
- If probes are in use, be sure they are differential probes which have no ground connection to the surged ground or to the equipment under test.

---

<sup>1</sup> Power-follow is a condition where the Surge event causes a low-impedance path which full mains current may then flow through. One example of this is a gas-tube arrester, which maintains a high impedance until a surge event switches it to a low-impedance state; the low-impedance state is maintained until the mains voltage drops below a critical threshold. Similar effects can be seen due to electrical arcs or exploded components.

- 
- The safety socket surge outputs are gold-plated. To ensure that the connectors will not deteriorate over time, always use gold-plated mating connectors.

## Safety Concerns During Surge Testing

Surge testing is hazardous. The equipment under test (EUT) can ignite, possibly explosively. Noxious, toxic and sometimes fatal fumes can be generated by the burning equipment. Accumulated gases may ignite explosively (i.e., *flashover*).

In an environment where surge testing takes place, it is absolutely crucial that these minimum safety precautions be taken:

- Surge testing should be performed only by properly trained test personnel who are experienced in conducting such tests, or be observed and supervised by such experienced personnel. No person subject to heart or neurological conditions should be allowed to conduct surge tests. Persons with pacemakers should not be allowed in or near the area where testing is conducted.
- Never leave a procedure or a test setup unattended.
- All personnel working in the area must be shielded with appropriate eye protection, body protection and electrical protection. They should not be allowed to work in a direct line of a possible explosion of the equipment under test.
- The test area should be a clear and unobstructed environment dedicated to such tests.
- The test area should be equipped with ventilating hoods and blowers to remove gases that may be caused by exploding or burning components.
- The test area should have nonflammable walls and floors plus shielding to contain exploding parts and flames.
- There must be fire extinguishers certified for use in electrical and chemical fires readily available at the test site. **DO NOT USE WATER TO EXTINGUISH AN ELECTRICAL FIRE.**
- All flammable materials and debris must be outside the test area, and the area must be well marked, preferably by physical barriers, to prevent accidental intervention by non-test personnel while a test is in progress.

---

## Inappropriate Uses

The **EMCPro** must be kept within the specified environmental limits of the operating requirements. This includes not using the **EMCPro** in condensing humidity.

The unit must not be operated by wearers of electronic life-support equipment. Personnel with pace-makers, heart problems, nervous disorders, and similar problems should not be allowed to operate the **EMCPro** or be present during ESD testing.

The ESD probe is capable of giving an unpleasant shock -- it is not intended for use as a shock prod, "cattle prod", or as any device designed to shock people or animals.

There are no User Serviceable parts inside; do not remove covers.

---

## Description

The **EMCPro** is an advanced EMC immunity test system developed by KeyTek in response to manufacturers' demands for a mid-range, low cost, multi-capability test system. The **EMCPro** is easily configured to meet today's immunity standards required for CE Marking and compliance requirements. In addition, **EMCPro** capabilities go well beyond the required test levels for the CE Mark.

The **EMCPro** performs compliance level testing requirements for IEC, UL, ANSI, ETSI and beyond. The **EMCPro** allows users to perform compliance testing to the following standards:

IEC 1000-4-2	ESD	UL 864
IEC 1000-4-4	EFT	ANSI/IEEE C62.41
IEC 1000-4-5	Combination and Telecom Wave Surge	EN 50082-1 EN-50082-2
IEC 1000-4-8	Power Frequency Magnetic Fields	CCITT K17, K20, K21 ETSI
IEC 1000-4-9	Pulse Magnetic Fields	UL 1449
IEC 1000-4-11	Dips and Interrupts	
IEC 1000-4-12	100kHz Ring Wave	

Users may operate the **EMCPro** via KeyTek's easy to use Windows-based PC software, **CEWare**, or from the front panel. **CEWare** provides simple, straight forward pre-programmed test sequences ideal for the novice user; yet is sophisticated enough to allow an advanced user to develop and save custom test sequences for future testing.

Users may configure the **EMCPro** from a single test capability to up to seven capabilities in a single unit. When test requirements change, or as standards evolve, upgrading is a simple matter of adding appropriate options or accessories offered by KeyTek to their current **EMCPro**.

One System, One Vendor, One Solution.

The **EMCPro** system offers the highest test levels and the widest selection of testing capabilities in a low-cost complete system solution.

---

# Installation

## Unpacking Instructions

### **EMCPro Assembly**

The **EMCPro** requires two people for unpacking. Check the packaging materials and follow any special unpacking instructions shipped with your unit. The **EMCPro** comes fully assembled.

Save all shipping materials (shipping boxes, foam pieces, bags, and special instructions) for possible future shipments. The original shipping materials must be used whenever the **EMCPro** is returned for calibration or service.

Carefully check all shipping materials for accessories which may be packaged with the **EMCPro**.

### **Computer Assembly**

If your system includes a computer: Unpack the computer and accessories. Verify that the voltage settings of the computer and monitor match your mains voltage.

## Handling, Transportation, Storage

Save all shipping materials (shipping boxes, foam pieces, bags, and special instructions) for possible future shipments.

The **EMCPro** requires two people for unpacking. Follow the instructions in the **INSTALLATION** section of this manual and any special instructions shipped with the unit.

Issues related to transportation of **EMCPro** models are identical to those for installation; the weight of the unit requires that two people help in packing and movement. When packing the unit for transportation the original shipping materials should be used, or new materials of equivalent strength and durability.

An optional transport case -- **PRO-CASE** -- is available for the unit.

For long storage intervals, unplug the power cords of the instrument and cover the instrument to protect from dust and liquid spills.

## Cabling and Interconnections


The **EMCPro** has two AC Mains cordsets which plug into the rear of the unit. One, the Systems Power input, powers the circuitry of the **EMCPro**. The second, the EUT Power input, powers the front panel mains connector and the Equipment Under Test. The cordsets used should be the right-angle cordsets supplied with the unit to prevent damage to the cordsets when moving the **EMCPro**.

The FiberCom option connects the **EMCPro** to an external computer running the **EMCPro** application software under Windows™ 3.x or Windows-95™. The FiberCom option (CM-SW) includes a small module, the FC-11, a short RS-232 cable with a 9-pin D-shell connector, and a fiberoptic cable with a duplex modular connector. The RS-232 connector connects to your computer. The fiberoptic cable connects to the **EMCPro** front panel; this connector is polarized and can only be inserted in one orientation: with the small tab on the connector facing right. Do not force the connector. The FiberCom option derives power from the RS-232 port of the computer -- no external power source is required.<sup>2</sup>


The optional ESD probe connector attaches to the front panel. This connector is polarized and can only be inserted in one orientation: align the flat of the connector plug with the flat of the front panel opening. Do not force the connector.

### Direct Current Power to EUT

The **EMCPro** can accept a Direct Current (DC) power source at the EUT input and provide it to the EUT output. When connecting to DC it is important to note the assignment of EUT inlet and outlet connectors.

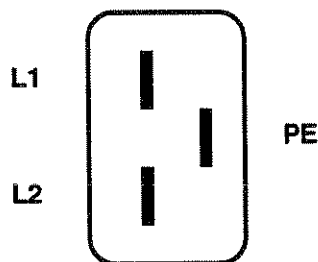

EUT Mains Inlet, Panel Wiring  
The IEC Inlet connector is wired,  
L1 top, L2 bottom, PE center.

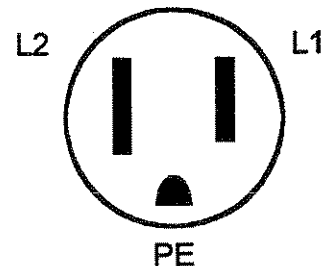

EUT Mains Outlet, Panel Wiring  
Regardless of nationality, the outlet is always  
wired, L2 left, L1 right, PE center.

For DC use L1 and L2 should be used for voltages or voltage and return; the PE connection should be used for return only. Note that PE will be connected to chassis during surge testing.


<sup>2</sup> Some computers use a low-power RS-232 driver with a reduced drive voltage. If the FiberCom fails to work with a computer, an external supply should be used [KeyTek part #02-701-695-00 (USA) and 62-050-415-00 (European)].



---

## AUX IN Connector to PQF

On the rear panel of the **EMCPro** are four safety socket outputs for the PQF Aux function.

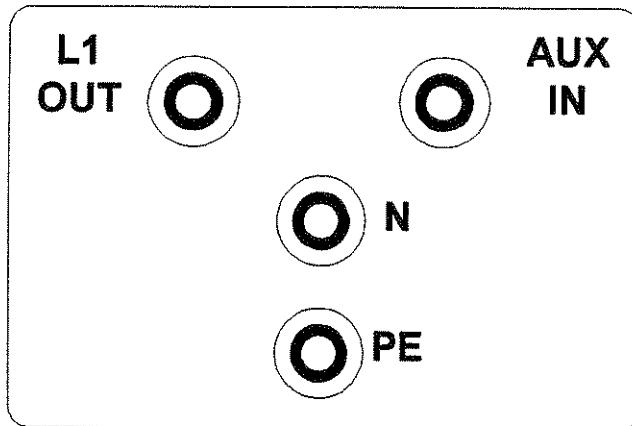

### L1 OUT, N, and PE

These connections are provided to the user, for connection of an external transformer or Variable-transformer, which may be used to derive an AUX IN voltage.

### AUX IN

The AUX IN connection is wired into the PQF circuitry, to allow the user to provide an AC voltage other than the standard, 0%, 40%, or 70% voltages.

When using the Auxiliary input, note the following:

- The L1 and N connections provide the EUT Mains voltage as an output. These connections are internally protected at 16 amperes by a self-resetting thermal breaker.
- L1 and N should not be connected to a source; these terminals are outputs -- not inputs.
- The protection for L1 and N is self-resetting; in the event of a fault these outputs will reset automatically. These lines should not be connected to circuitry which will become a hazard if energized unexpectedly.
- The AUX IN voltage must be AC, within the range of zero to 318Vac, 50/60Hz. Do not connect AUX IN to direct current.
- The AUX IN may be greater than EUT IN, but may not exceed the EUT IN by more than 20%.
- If AUX IN is derived from a source other than the L1 and N connections provided, the user should fuse or protect the AUX IN line for a current less than or equal to the rating of the **EMCPro** -- 16 amperes.

## Interlock Connector

The optional interlock allows the user to connect a remote switch which, when open, removes all AC and high-voltage from the **EMCPro** front panel outlets, and disables the ESD head.

A spare interlock connector is provided in the accessories kit for the **EMCPro**. To use this connector, wire your cable from the connector TIP and RING contacts, and provide a simple switch or contact closure at the other end of the cable.

- 
- The interlock operates from an internal, +5V, 20mA, logic level signal. Do not connect the interlock to a power source.
  - Use a cable with voltage rating of twice the voltage rating of your EUT.
  - Route the interlock cable away from the EUT output and the EUT.
  - DO NOT connect the interlock within the EUT, or to circuitry tied to the EUT.
  - DO NOT use a momentary switch to control the interlock. It is latched, internally, but a momentary switch may not be open long enough to activate the latch.

### Stop Test Input Connector

A coax connector is provided on the front panel to allow remote interruption of an **EMCPro** test. This connector is internally connected to a 5 volt reference; if this connection is shorted -- coax center connector to shield -- during a test, the **EMCPro** will treat this event the same as if the STOP button is pressed -- halting the present test. If remote logging is enabled, this event will be logged as a user interruption of the test. While this connection is shorted, the **EMCPro** cannot be programmed and no test can be started. The minimum duration of the short must exceed 0.15 second.



#### CAUTION

You should not connect a voltage source or generator to the Stop Test Input Connector; doing so may damage the **EMCPro**

---

### Voltage and Current Monitor Connectors

Two coax connectors are provided on the front panel to monitor surge voltage and current, or mains voltage and current via external equipment (e.g. oscilloscopes or voltmeters). The mode of these outputs, and the voltage scaling, changes with the settings of the **EMCPro**.



#### CAUTION

You should not connect a voltage source or generator to the IMon or Vmon connectors; doing so may damage the **EMCPro**

---

### PQF Synchronization Connector

A coax connector is provided on the front panel to allow synchronization of external equipment (e.g. oscilloscopes) with the PQF event. This connector will output a 5 volt pulse at the start of a PQF event, with the pulse duration equal to the duration of the PQF event.



#### CAUTION

You should not connect a voltage source or generator to the PQF Synchronization Connector; doing so may damage the **EMCPro**

---

### Capacitive Clamp Cable

A 1 meter long stereo phono plug cable and a 1 meter HN-coaxial cable are provided with the CM-CCL, and CM-CCLC options. The coax cable is screwed onto the **EMCPro** coax output, and to either end of the CM-CCL or cable clamp. The unused coaxial connector on the opposite

---

end of the cable clamp should be left unterminated, or can be used with an optional, coaxial probe to monitor the delivered voltage.

The CM-CCLC cable clamp includes an interlocked safety cover. By connecting the stereo phono plug cable between **EMCPro** and either end of the cable clamp, the **EMCPro** will operate only if the cover of the cable clamp is properly seated. The unused interlock jack on the opposite end of the cable clamp can be used to wire to additional interlock switches.

### **I/O and Telecommunication Cables**

The Combination Surge wave and Ring wave can be connected to I/O communication lines (unbalanced datalines) using the optional **CM-I/OCD** coupler and cable. The cable is connected between the white and grey safety sockets of the **EMCPro** (labeled 1.2/50) and the white and grey safety sockets of the **CM-I/OCD**.

The optional 10/700us wave can be connected to telecommunication lines (balanced datalines) using the optional **CM-TELCOM** coupler and cable. The cable is connected between the white and grey safety sockets of the **EMCPro** (labeled 10/700) and the white and grey safety sockets of the **CM-TELCOM**.

### **CM-3CD Cables -- Connections to Three-phase Mains**

The Combination Surge wave (and optional Ring wave) can be connected to a three-phase mains for Surge and EFT testing using the optional **CM-3CD** coupler and cable. The Surge cable is connected between the white and grey safety sockets of the **EMCPro** (labeled 1.2/50) and the white and grey safety sockets of the **CM-3CD**. The EFT cable is connected between the HN-coax connector of the **EMCPro** and the HN-coax connector of the **CM-3CD**.



#### **CAUTIONS**

**Do not connect the CM-3CD cables to the Telecom wave (labeled 10x700) safety sockets. Do not attempt to run Diagnostic tests or Power Frequency Magnetic Field tests or Pulsed Magnetic Field tests while connected to a CM-3CD.**

**Damage to the EMCPro may result!**

**Disconnect the surge cable from both units when not testing.**

---

### **Magnetic Coil Connections**

An **EMCPro** -to-coil cable is provided with the CM-HCOIL option. The **EMCPro** -end of the cable is plugged into the front-panel safety sockets, labeled "To H-Coil." The coil end of the cable plugs into the sockets on the coil.

### **Other Cables**

The **EMCPro** accessories kit includes safety socket connectors and an interlock connector which the user may use to fabricate special test cables. When fabricating cables, always use wire rated for twice the peak, pulse voltage present during testing.

---

## Electrical Supply Requirements

### System Power

The **EMCPro** will automatically configure for your AC Mains voltage, choosing one of two voltage ranges:

100 - 120 Vac, 50/60 Hz

220 - 240 Vac, 50/60 Hz

### EUT Power

The **EMCPro**, EUT power inlet can accept input voltages from 50 - 240 Vac, 50/60 Hz.

**HOWEVER**, the rating of the **EMCPro** is limited by the EUT mains connector rating, as follows:

PRO-BASE-USA	15A, 120 Vac
PRO-BASE-BRI	13A, 250 Vac
PRO-BASE-EUR	16A, 250 Vac

The AC power source for the EUT must have adequate capacity for full power-follow<sup>3</sup> in the event that testing causes an equipment failure. Using a supply without sufficient capacity may result in a failure being masked.

Acceptable power sources include:

- A dedicated branch circuit.
- The dedicated output of a motor-generator (MG) set.
- The output of a properly installed isolation transformer.

### Use of the **EMCPro** with Ground-Fault Interrupters (GFI)

Problems may result when using the **EMCPro** on AC mains protected by Ground-Fault Interrupters (GFIs). Surging the EUT, with a coupling mode to PE (L1-PE, L2-PE, or L1&L2-PE) will cause the GFI to trip, causing an unexpected loss of AC power to the EUT.

The problem is due to the coupling network mandated by IEC 1000-4-5; this network connects the surge generator to the AC mains during the surge pulse, and creates a short pulse of mains current in PE, tripping the GFI. This problem only occurs during Surge events with a PE coupling mode selected.

---


<sup>3</sup> Power-follow is a condition where the Surge event causes a low-impedance path which full mains current may then flow through. One example of this is a gas-tube arrestor, which maintains a high impedance until a surge event switches it to a low-impedance state; the low-impedance state is maintained until the mains voltage drops below a critical threshold. Similar effects can be seen due to electrical arcs or exploded components.

---

There are two solutions to this problem:

- The first solution is to power the EUT from a source that does not have a GFI device installed. This solution may not be practical in some locations due to building codes or safety regulations.
- The second solution is to install an isolation transformer between the AC mains and **EMCPro**. The isolation transformer should be rated for *at least* 1920VA for 120VAC mains, or 3840VA for 220/240VAC mains. The transformer should be wired as diagrammed below.

Note that L2 - Neutral - is bonded back to PE at the output of the transformer.

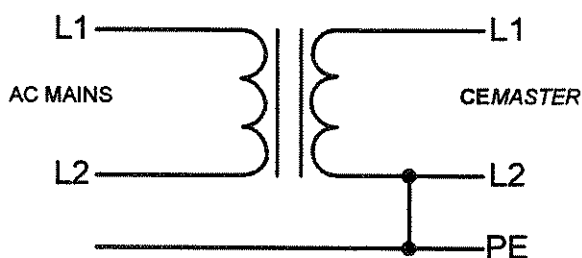

Proper Connection of an Isolation Transformer

**Note**

*A solid-state regulated line source such as an uninterruptable power supply (UPS) or a power frequency amplifier will generally not have the instantaneous capacity or full power-follow required for Surge and PQF testing, and therefore should not be used as the AC power source for any equipment being tested.*

---

## Physical Environment

**EMCPro** systems are intended for operation in a laboratory environment, protected from excess dust, humidity, and temperature.

- No condensing humidity or standing water on the floor or work surfaces.
- No significant dust or other contamination.

## Operating limits

Temperature:	15 - 40° C
Humidity:	10 - 85%, non-condensing
Altitude:	8,000 feet max.

## Storage limits

Temperature:	0 - 60° C
Humidity:	10 - 90%, non-condensing
Altitude:	8,000 feet max.

### Note:

---

If an **EMCPro** system has been subjected to temperature or humidity outside of the normal operating limits, for a period exceeding four hours, place the system in an environment of the proper temperature and humidity and allow the system to stabilize in that environment for a period of 24 hours; during stabilization, the unit should be unpacked, but not powered nor operating.

The **EMCPro Pro-ESD** option may require as much as 48 hours stabilization time if the period exceeding the humidity limits exceeds four hours.

---

---

## Test Area Considerations and Site Preparation

Conduct pulsed EMI testing under sound laboratory conditions. Verify the following:

- No condensing humidity or standing water on the floor or work surfaces.
- No significant dust or other contaminants .
- Clear and unobstructed vision.
- Adequate ventilation, including ventilating hoods and blowers to remove gases.
- Nonflammable walls and floors.
- Barriers surrounding the EUT to contain exploding parts and flames.
- Appropriate fire extinguishers for electrical and chemical fires. **DO NOT USE WATER TO EXTINGUISH AN ELECTRICAL FIRE.**
- No flammable materials or debris inside the test area. The area must be well marked, preferably by physical barriers.
- Keep unauthorized personnel out of the area during testing.

Allow at least six inches clearance from the wall or other equipment on both sides of the instrument for proper air flow. The system must be mounted on a level surface.

For EFT testing the **EMCPro** should be mounted on the floor, on the ground reference plane. For other testing, the **EMCPro** may be placed on a table that can support the weight of the unit. It may also be placed on a sturdy cart. However, since the unit is heavy, make certain that the instrument and cart combination is stable, and cannot be easily tipped - particularly if the wheels strike a bump on the floor such as the edge of a rug, a pebble or a small piece of hardware.

## Special Considerations for Surge Testing

Pulsed-EMI testing is best done in an area cleared of obstructions. Clearly mark the boundaries of the area.

There is the possibility that the surge may flash over to circuits or metal objects not directly under test, and that components in the equipment being tested may explode or ignite under the stress of the surge test. Whenever possible, enclose the equipment under test within a fireproof and explosion-proof barrier having insulation capable of withstanding at least twice the maximum surge voltage.

Never allow direct line-of-site view of components that may explode or ignite. If visual observation is required, use a robust transparent barrier of suitable thickness for protection.

Pulsed-EMI testing should only be carried out by fully trained personnel who are informed of the hazards of such testing, and who have full control over all of the test equipment in the area.

The **EMCPro** contains orientation-sensitive components, and will only perform Surge testing when operated in a horizontal position; for accurate, repeatable results the **EMCPro** should be level, and should be used in a location free from vibration.

---

## ✓ Special Considerations for EFT Testing

### NOTE


**While the possibility of component destruction is less of a concern during EFT testing, it should not be ignored.**

EFT testing involves the use of very high frequency pulses. For this reason the testing standards specify the use of a ground reference plane in the area where EFT testing is performed. In addition, the standards specify the minimum and maximum spacings among the various equipment present in the test area.

This device complies with the requirements of the EMC Directive, 89/336/EEC, as stated in the declaration of Conformity. However, EFT test pulses are by nature an interference test and can therefore create a possible source of disturbance to other electronic equipment that is not intended for test. This device should be used in an environment free of other equipment that could be affected by these emissions, or in a shielded room.

The floor of the test area is to be covered with copper or aluminum with a minimum thickness of 0.01 inch, which must be bonded to building Protective Earth (PE) ground. In addition, the cabinet of the **EMCPro** must be directly tied to the ground reference plane. Provision for a mounting bracket is made on the rear and bottom of the **EMCPro** and the bracket and screws are provided.


Grounding Bracket



Rear View


EFT Grounding Bracket Location



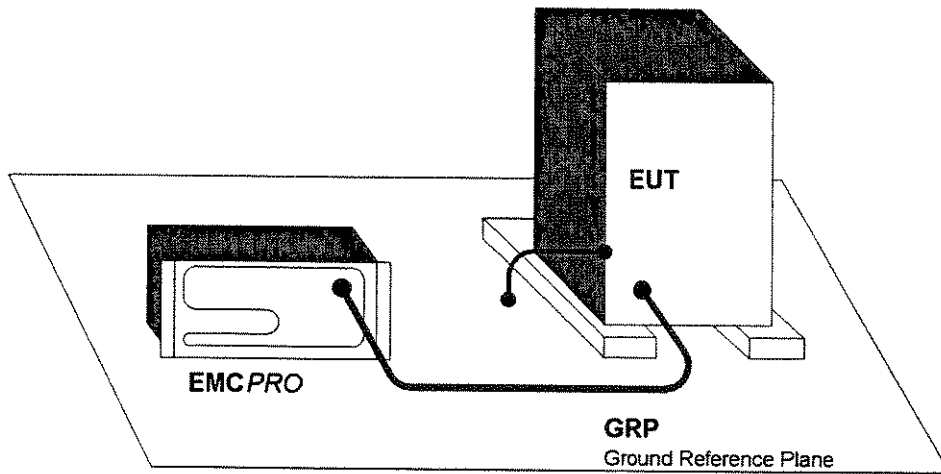


EFT Connection to Equipment Under Test for Floor-standing EUT

When used with table-top equipment, the equipment should be placed on an insulating table of 0.8 meters height.

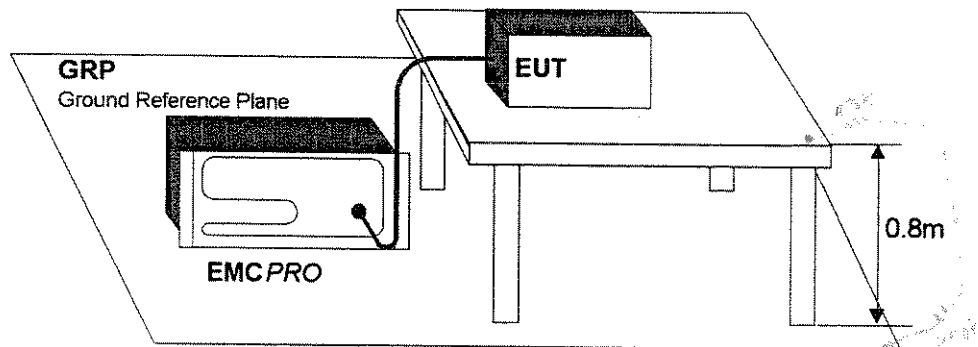

EFT Connection to Equipment Under Test for Table-top EUT

Data and signal cables are tested using the EFT Capacitive Coupling Clamp (CM-CCL). When performing these tests, the EUT and any auxiliary equipment should be powered from the **EMCPro** EUT output, to provide isolation between the test setup and building power mains. The minimum spacing required between the clamp and the equipment in the test area is shown in the figure below.

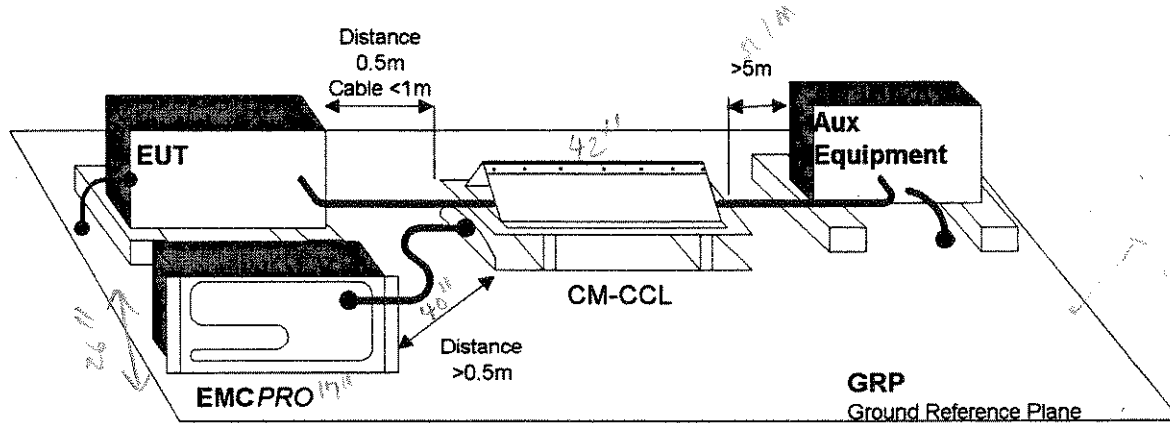

Use of the Capacitive Cable Coupler for EFT Testing

The **EMCPro** contains orientation-sensitive components, and will only perform EFT testing when operated in a horizontal position; for accurate, repeatable results the **EMCPro** should be level, and should be used in a location free from vibration.

---

## Special Considerations for ESD Testing

ESD testing involves the use of high-voltage, fast-rising pulses. For this reason the testing standards specify the use of a ground reference plane in the area where ESD testing is performed.

---

This device complies with the requirements of the EMC Directive, 89/336/EEC, as stated in the declaration of Conformity. However, ESD test pulses are by nature an interference test and can therefore create a possible source of disturbance to other electronic equipment that is not intended for test. This device should be used in an environment free of other equipment that could be affected by these emissions, or in a shielded room.

---

IEC 1000-4-2 requires the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is  $1 \text{ m}^2$ , the exact size depending on the dimensions of the EUT; the ground plane shall extend beyond the EUT by at least 0.5 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

For ESD testing, the **EMCPro** need not be connected to the ground plane.

The EUT shall be positioned at least 1 m from walls and any metallic structures.

For table-top equipment, a non-conducting table 0.8 m high is placed on the ground plane. A ground plane (HCP) 1.6 m by 0.8 m will be put on the table, and the EUT and any cables shall be placed on an insulating support 0.5mm thick placed on top of the HCP. The HCP shall connect to the ground reference plane with a resistive cable with two, 470,000 ohm resistors, one resistor at each end of the cable.

## Special Considerations for Pulsed Magnetic Field and Power-Frequency Magnetic Field Testing

IEC 1000-4-8 and IEC 1000-4-9 require the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is  $1 \text{ m}^2$ , the exact size depending on the dimensions of the EUT; the ground plane shall extend beyond the EUT by at least 0.5 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

For Magnetic Field testing, the **EMCPro** need not be connected to the ground plane.

The EUT is placed on the ground reference plane, on an insulating support 0.1 meter thick.


The coil and EUT shall be positioned at least 1 meter from walls and metallic objects.

---

This page intentionally left blank.

# Introduction

The features of the **EMCPro** are broken into five, major groups: the System Interconnections, the Equipment-Under-Test Connections, the Monitoring and Control Connections, the Rear-Panel Auxiliary Connections, and the User Interface.

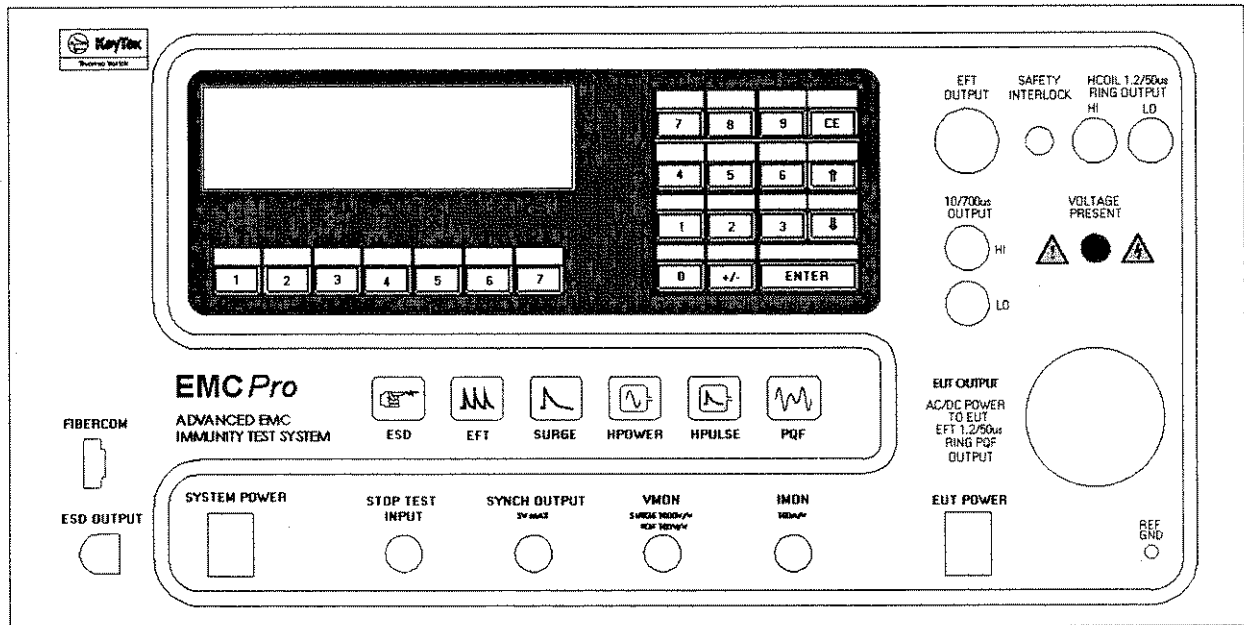



## EMCPro System Interconnections -- ESD and Computer Interface

FIBERCOM




SYSTEM POWER

ESD OUTPUT



On the left, bottom side of the **EMCPro** front panel are connectors for the FiberCom serial port, the ESD test probe, and the power switch for the **EMCPro**. Note that both connectors are polarized. On the FiberCom connector the small tab on the connector faces right. On the ESD probe connector, align the flat of the connector plug with the flat of the front panel opening. Do not force the connectors.


## Connection to the Equipment Under Test

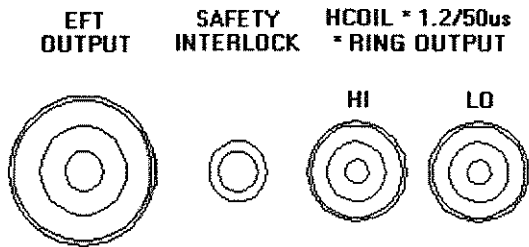

The EFT output coax connects to the Capacitive Cable Clamp or three-phase coupler. This coax is also used for waveform verification.

The Safety Interlock connector allows the user to connect a remote switch which, when open, removes all AC and high-voltage from the **EMCPro** front panel outlets, and disables the ESD head.


The Safety socket outputs, at upper right, couple 1.2/50us surge pulses to the magnetic coil or communication lines, and can be used for component testing. These sockets are also used to provide power frequency magnetic field output to a test coil.

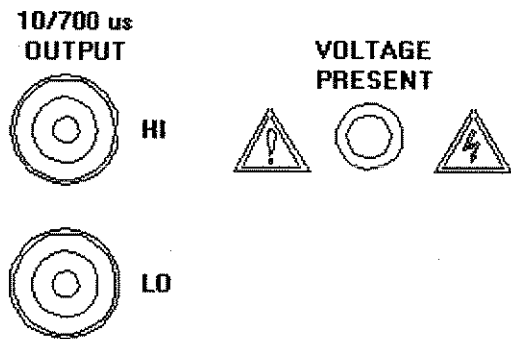


The Safety socket outputs, in the middle of the **EMCPro**, output the 10/700us telecom wave; this waveform is available for component testing and for coupling to Telecom lines -- it is not for use with AC Mains and AC Mains couplers.

The Voltage Present LED is lit when the AC Mains outlet is energized or when high voltage is present

EUT OUTPUT  
AC/DC POWER  
TO EUT  
EFT \* SURGE \* PQF  
OUTPUT

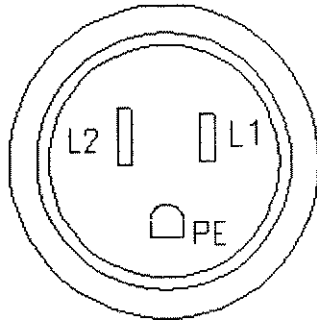

EUT POWER



REF GND



The EUT Power connector provides AC Mains to the Equipment Under Test.

The EUT Power switch energizes the EUT Power connector.

---

For safety, a positive, operator-action is required to energize the EUT; i.e. if the EUT power switch is ON when the **EMCPro** is first turned on, the switch must be toggled OFF and then ON to energize the EUT Power connector.

---

The Reference Ground Connector is a chassis connection provided for waveform verification of the EFT waveform; it is not used during normal testing.

### Interlock Connector

The optional interlock allows the user to connect a remote switch which, when open, removes all AC and high-voltage from the **EMCPro** front panel outlets, and disables the ESD head. This is useful to establish a safety perimeter for protection of personnel.

- The interlock operates from an internal, +5V, 20mA, logic level signal. Do not connect the interlock to a power source.
- Route the interlock cable away from the EUT output and the EUT. DO NOT connect the interlock within the EUT, or to circuitry tied to the EUT.
- DO NOT use a momentary switch to control the interlock. A momentary switch may not be open long enough for the **EMCPro** firmware to latch the interlock event.

---

## Monitoring and Control Connections

Four coax connectors are provided along the bottom, front of the **EMCPro** for access to the internal monitoring features, and control of tests.

### Stop Test Input Connector

A coax connector is provided on the front panel to allow remote interruption of an **EMCPro** test. When the coax center connector is shorted to shield the **EMCPro** will treat this event the same as if the STOP button is pressed -- halting the present test. If remote logging is enabled, this event will be logged as a user interruption of the test. While this connection is shorted, the **EMCPro** cannot be programmed and no test can be started. The minimum duration of the short must exceed 0.15 second.

This connector is internally connected to a 5 volt reference. You should not connect a voltage source or generator to the Stop Test Input Connector; doing so may damage the **EMCPro**.

### VMon and IMon -- Voltage and Current Monitor Connectors

Two coax connectors are provided on the front panel to monitor surge voltage and current, or mains voltage and current via external equipment (e.g. oscilloscopes or voltmeters). The mode of these outputs, and the voltage scaling, changes with the settings of the **EMCPro**.

Operating Mode	Vmon		IMon	
	Vmon Source	Vmon Scale	IMon Source	IMon-Scale
Surge, PMF	Surge Out	1V / 1000V	Surge Out	1V / 200A
Main Menu PQF, PFMF, ESD	EUT Mains Out	1V / 100V	EUT Mains Out	1V / 200A
EFT	No output	No output	No output	No output

The IMon output has a low impedance of 1 ohm; for reasonable accuracy this output should only be used with measuring instruments with input impedance exceeding 10,000 ohms.

The VMon output -- when measuring surges only -- has an impedance of fifty ohms. Connecting this output to an instrument with fifty ohms input impedance will minimize transmission line effects, and reduce the voltage scaling by a factor of two. The VMon output -- when measuring EUT Mains -- should not be terminated by fifty ohms, and should only be used with instruments with input impedance exceeding 10,000 ohms.

The typical accuracy of all outputs is  $\pm 10\%$ .

Voltage and current monitors are internal to the **EMCPro**; this is very convenient but results in some limitations. The voltage monitors are affected by the resistance and inductance of internal and external wiring, and by the close proximity to surge discharges exceeding 300 joules of energy.



- 
- The voltage monitor is a good approximation of the open-circuit waveform, but may show distortions when measuring the waveform into an EUT -- or a device -- where low-impedances to ground or non-linear impedance characteristics (MOVs, gastubes, etc.) may cause distortion of the monitor waveform. Such distortions are a characteristic of the voltage monitor -- the actual surge waveform will not show this distortion.

The voltage monitor is an approximation of the open-circuit waveform internal to the **EMCPro**: due to resistance and inductance of internal and external wiring, the voltage delivered to the EUT may differ.

- Noise spikes are typical on the rising edge of the voltage monitor waveform. This noise may make it difficult to measure rise time.

These noise spikes are a characteristic of the voltage monitor -- the actual surge waveform will not show this noise.

- For surge waveform verification, the use of external voltage probes is recommended.
- The voltage monitor uses high-voltage relays to switch channels; this may cause false triggering of oscilloscopes at the beginning of a test (before the pulse), after a test, and when selecting or deselecting Surge tests from the Main Menu. These effects are caused by relay switching, and are not an indication that pulses are being produced.
- When performing surge tests (1.2/50, 10/700, Ringwave, PMF) the current monitor will read zero before and after the surge event. During the surge event, the monitor will be switched to the appropriate output (front panel, or EUT AC outlet) and will read the surge current. When surging to the EUT AC outlet, the current monitor will read the surge current, superimposed on the EUT mains current; this may increase or decrease the peak surge current, by the amount of the mains current at the time of the surge.

The current monitors are less affected by the resistance and inductance of internal and external wiring, and give very accurate response.



**CAUTION**

You should not connect a voltage source or generator to the **IMon** or **Vmon** connectors; doing so may damage the **EMCPro**

---

**PQF Synchronization Connector**

A coax connector is provided on the front panel to allow synchronization of external equipment (e.g. oscilloscopes) with the PQF event. This connector will output a 5 volt pulse at the start of a PQF event, with the pulse duration equal to the duration of the PQF event.



**CAUTION**


You should not connect a voltage source or generator to the **PQF Synchronization Connector**; doing so may damage the **EMCPro**

---

---

## Rear-Panel Auxiliary Connections

On the rear panel of the **EMCPro** are four safety socket outputs for the PQF Aux function.

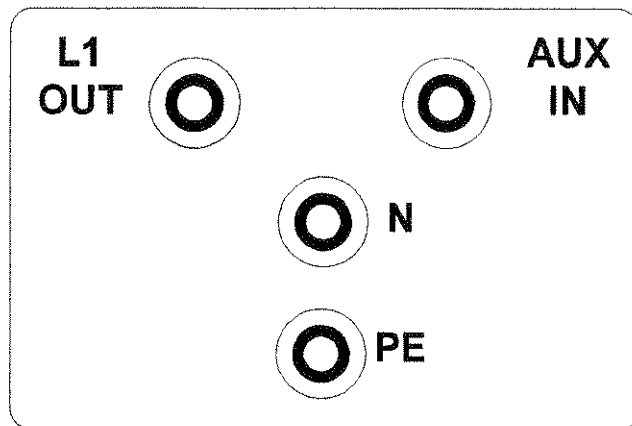

### L1 OUT, N, and PE

These connections are provided to the user, for connection of an external transformer or Variable-transformer, which may be used to derive an AUX IN voltage.

### AUX IN

The AUX IN connection is wired into the PQF circuitry, to allow the user to provide an AC voltage other than the standard, 0%, 40%, or 70% voltages.



When using the Auxillary input, note the following:

- The L1 and N connection provides the EUT Mains voltage as an output. These connections are internally protected at 16 amperes by a self-resetting thermal breaker.
- L1 and N should not be connected to a source; these terminals are outputs -- not inputs.
- The protection for L1 and N is self-resetting; in the event of a fault these outputs will reset automatically. These lines should not be connected to circuitry which will become a hazard if energized unexpectedly.
- The AUX IN voltage must be AC, within the range of zero to 318Vac, 50/60Hz. Do not connect AUX IN to direct current.
- The AUX IN voltage may exceed the EUT IN, but may not exceed the EUT IN by more than 20%.
- If AUX IN is derived from a source other than the L1 and N connections provided, the user should fuse or protect the AUX IN line for a current less than or equal to the rating of the **EMCPro** -- 16 amperes.

---


## User Interface

The **EMCPro** front panel includes a liquid crystal display with seven function keys, and a 15-key keypad to the right of the display.

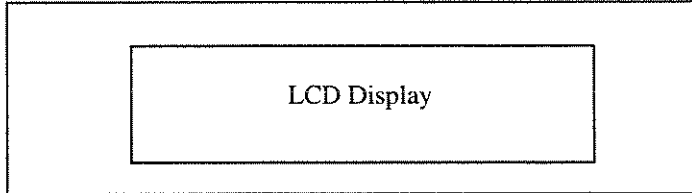

The liquid crystal display and seven function keys provide quick user input. The function keys are mapped to the bottom line of the display. Pressing a function key executes that command.

Typical commands are EXIT (go back one menu), RUN, and scroll through menu selections.

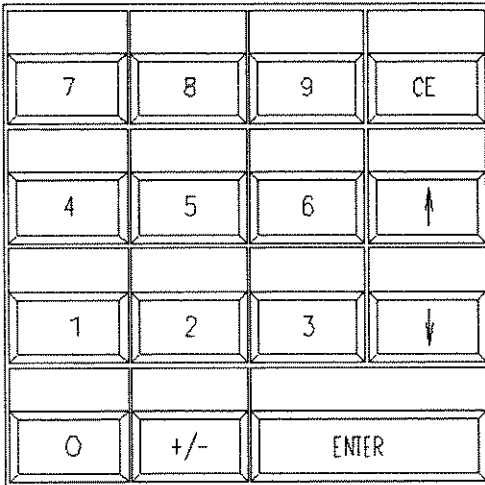

The numeric keypad is used to select menu items and enter numeric data into edit fields. The keys are defined as follows:

- 0 thru 9     Enter numeric data or select menu items
- +/-         Change polarity
- CE          Clear Entry; erase a numeric field
- ENTER      Accept the current input or menu item
- ↑↓          Scroll through selection list boxes, and increment or decrement numeric fields



```

| SRG 1.2/50 |||EUT OFF|
1. User defined      6. Class 2 Full
2. Class 2 Fast     7. Class 3 Full
3. Class 3 Fast     8. Class 4 Full
4. Class 4 Fast
5. Class 1 Full

||  ||  ||  ||  ↑  ||  ↓  ||EXIT

```

**Parameter Definition Menu**

After selecting either the User-Defined test option, or a pre-programmed test, a **Parameter Definition Menu** opens. The **Parameter Definition Menu** has edit fields, for waveform, voltage, etc. To change a field you first move the highlight bar to that field, using the function keys. After selecting a field there are different editing steps, depending on the type of field.

- List fields have a limited number of specific values. An example is the line synch field which can accept "L1" or "RAND". With a list field selected, the value is changed by using the keypad arrow keys to scroll through the options.
- Numeric fields are edited by typing a value at the keypad. The keypad input fills the available field from right to left (If the field allows a decimal place, such as "##.##" and thus a value between 0 and 99.99, to enter a value of 10, press "1", "0", "0", "0"). Press "+/-" after the number to make it negative. Press ENTER or move the highlight bar to another field to accept the value; the value must be accepted before a test can be run.
- Some fields combine Numeric and List fields. When selected, the keypad arrow keys change the list portion (L1,RND) and the keypad number keys replace the numeric value.

When all entries have been made and accepted the test can be started by pressing the F1 key -- the RUN function key. To exit this menu without starting a test, press the F7 key -- the EXIT function key.

```

| SURGE: USER DEF |||EUT OFF|
Waveform ..... 12 Ohm
Voltage ..... +2000 V
Output: Coupling ... MAINS:L1,L2/PE
Phase Sync: Angle .. L1:180 deg
Number of Tests ... 500
Time Between Tests 60 s
RUN ||  ||  ||  ||  ↑  ||  ↓  ||EXIT

```

When a pre-programmed test has been selected, many parameters assume default values and cannot be changed by the user; these fields cannot be selected or highlighted. The fields for these parameters are replaced with an AUTO symbol.









The left column shows test information:

Status (charging, running, etc.)  
 Time (secs left in this test step)  
 Comm (local, remote)  
 Test (test n of total tests)

The Status bar indicates the active test; Surge, and the menu; RUN.

EUT status shows the front panel outlet is ON or OFF

```

| SURGE: RUN | ||||| | EUT ON | | | | |
|           | ||||| |         |
|           | ||||| |         |
| Status: Charging | +2000 V |
| Time: 37s | MAINS:L1,L2/PE |
| Test: 1/90 | L1:180 deg |
| Comm: Local | 3 |
|           | 60 s |
| STOP|| ||PAUSE|| || || ||
  
```

The STOP -F1- function key halts the test


The PAUSE -F3- function key pauses the test. Press F3 again to resume

The right column shows programmed test parameters: waveform, voltage, coupling mode, line synch, number of tests, and time between tests (or length of test).


Definition of the Run Screen Menu

## Map of Front Panel Menu Structure

The next three pages show the structure of the front panel menus.

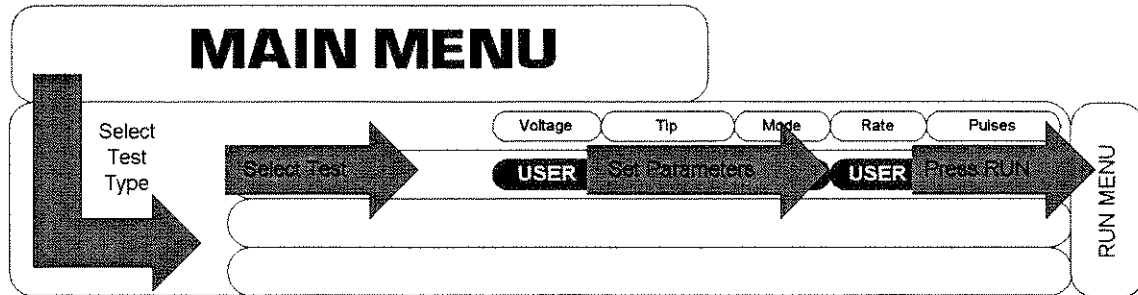

Selection Flow, from Main Menu through Test Menu, Parameter Definition Menu, and Run Menu

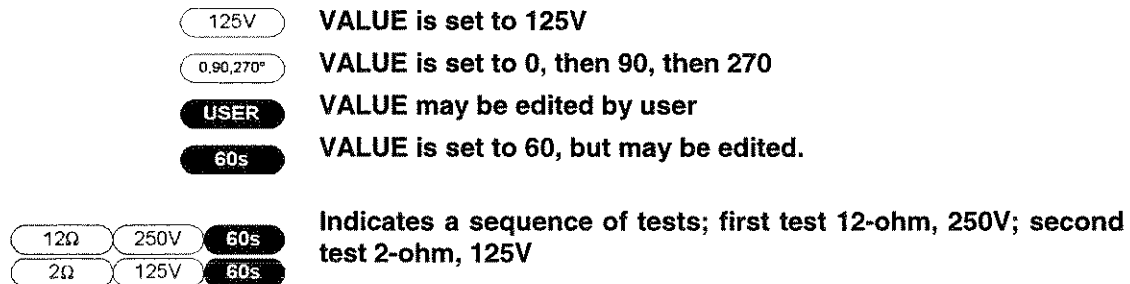

### LEGEND, MAP OF FRONT-PANEL MENUS

# MAIN MENU

1 EFT	USER DEFINED	Voltage	frequency	Coupling	Duration	RUN MENU		
	CLASS 1	±500V	5KHZ	L1,L2,PE	60s			
	CLASS 2	±1kV	5KHZ	L1,L2,PE	60s			
	CLASS 3	±2kV	5KHZ	L1,L2,PE	60s			
	CLASS 3	±4kV	2.5KHZ	L1,L2,PE	60s			
2 SURGE 1.2X50us	USER DEFINED	Waveform	Voltage	Coupling	Synch	Interval	nbr tests	RUN MENU
	CLASS 2 FAST	12Ω	1000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	500V	L1/L2	0.90,270°	60s	5+,-	
	CLASS 3 FAST	12Ω	2000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	1000V	L1/L2	0.90,270°	60s	5+,-	
	CLASS 4 FAST	12Ω	4000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	2000V	L1/L2	0.90,270°	60s	5+,-	
	CLASS 1 FULL	12Ω	500V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
	CLASS 2 FULL	12Ω	500V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		12Ω	1000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	500V	L1/L2	0.90,270°	60s	5+,-	
	CLASS 3 FULL	12Ω	500V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		12Ω	1000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	500V	L1/L2	0.90,270°	60s	5+,-	
		12Ω	2000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
	CLASS 4 FULL	2Ω	1000V	L1/L2	0.90,270°	60s	5+,-	
		12Ω	1000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
		2Ω	2000V	L1/L2	0.90,270°	60s	5+,-	
		2Ω	1000V	L1/L2	0.90,270°	60s	5+,-	
	CLASS 4 FULL	12Ω	4000V	L1/PE,L2/PE	0.90,270°	60s	5+,-	
2Ω		2000V	L1/L2	0.90,270°	60s	5+,-		
12Ω		4000V	L1/PE,L2/PE	0.90,270°	60s	5+,-		
2Ω		2000V	L1/L2	0.90,270°	60s	5+,-		
3 POWER FREQUENCY MAGNETIC FIELD	USER DEFINED	Coil Factor	Field Strength	Frequency	Duration	RUN MENU		
	4 ESD	USER DEFINED	Voltage	Tip	Mode	Rep Rate	Nbr Pulses	RUN MENU
	AIR 8kV	±8kV	AIR	USER	1pps	USER	RUN MENU	
	CONTACT 4kV	±4kV	CON	USER	1pps	USER	RUN MENU	
5 PQF	USER DEFINED	Level	Start Angle	Duration	Interval	Nbr Tests	RUN MENU	
	0% OPEN/5S	0%open	0°/180°	5s	USER	3/6	RUN MENU	
	0% SHORT/5S	0%short	0°/180°	5s	USER	3/6	RUN MENU	

Map of Front-Panel Menus, Page 1 of 2

5 PQF	40% 0.1S	40%	0°/180°	0.1s	USER	3/6	RUN MENU	
	70% 0.01S	70%	0°/180°	0.01s	USER	3/6		
	COMBINATION	0%open	0°/180°	5s	USER	3/6		
		0%short	0°/180°	5s	USER	3/6		
		40%	0°/180°	0.1s	USER	3/6		
		70%	0°/180°	0.01s	USER	3/6		
	Qualify 90°	Qualify 270°						
6 PULSE MAGNETIC FIELD	USER DEFINED	Coil Factor	Field Strength	Interval	nbr Tests		RUN MENU	
	CLASS 3	USER	100A/m	USER	5			
	CLASS 4	USER	300A/m	USER	5			
	CLASS 5	USER	1000A/m	USER	5			
7 SURGE (10x700)	USER DEFINED	Voltage	Interval	nbr Tests			RUN MENU	
	LEVEL 1 FAST	500V	USER	1				
	LEVEL 2 FAST	1000V	USER	1				
	LEVEL 3 FAST	2000V	USER	1				
	LEVEL 4 FAST	4000V	USER	1				
8 SURGE (Ring- wave)	USER DEFINED	Waveform	Voltage	Coupling	Synch	Interval	nbr tests	RUN MENU
	2kV 200A ANSI	200A	2000V	4 MODES	0,90,270°	60s	5+,5-	
	4kV 200A ANSI	200A	4000V	4 MODES	0,90,270°	60s	5+,5-	
	6kV 200A ANSI	200A	6000V	4 MODES	0,90,270°	60s	5+,5-	
	2kV 500A ANSI	500A	2000V	4 MODES	0,90,270°	60s	5+,5-	
	4kV 500A ANSI	500A	4000V	4 MODES	0,90,270°	60s	5+,5-	
	6kV 500A ANSI	500A	6000V	4 MODES	0,90,270°	60s	5+,5-	
	Lev1 200A IEC	200A	500/250V	4 MODES	0,90,270°	60s	5+,5-	
	Lev2 200A IEC	200A	1k/500V	4 MODES	0,90,270°	60s	5+,5-	
	Lev3 200A IEC	200A	2k/1kV	4 MODES	0,90,270°	60s	5+,5-	
	Lev4 200A IEC	200A	4k/2kV	4 MODES	0,90,270°	60s	5+,5-	
	Lev1 500A IEC	500A	500/250V	4 MODES	0,90,270°	60s	5+,5-	
	Lev2 500A IEC	500A	1k/500V	4 MODES	0,90,270°	60s	5+,5-	
	Lev3 500A IEC	500A	2k/1kV	4 MODES	0,90,270°	60s	5+,5-	
Lev4 500A IEC	500A	4k/2kV	4 MODES	0,90,270°	60s	5+,5-		
10 SYSTEM	PARAMETERS	DIAGNOSTICS						
	ACCESS CODE	VERSIONS						

Map of Front-Panel Menus, Page 2 of 2

---

## Programming the EMCPro from a Personal Computer

When purchased with the **PRO-SW** option, the **EMCPro** may be programmed and controlled from a Personal Computer (PC) running Windows™.

The PC software gives full access to all the features and capabilities of the **EMCPro**, including running a single test, running a pre-defined test sequence, and running diagnostics.

In addition, the PC software allows the user to:

- Create tests and easily edit them.
- Chain tests into a test sequence. A test sequence can be constructed from a single test type (e.g. Surge) or can combine test types (e.g. do one Surge test followed by one EFT test, etc.).
- Store and recall tests and test sequences to disk.
- Print or file text descriptions of tests and test sequences (for inclusion in reports).
- Log a test -- print or file what tests are executed.

Full instructions for the software are described in the **CEWare™** section.

---

# Running Tests

## STANDARDS OVERVIEW

The European Union's EMC Directive requires that electronic and electrical products be tested for immunity to both man-made and natural phenomena and to insure that products do not emit unintentional signals that may interfere with the continued, reliable operation of other products.

Compliance with the EMC Directive requires that products be tested in accordance with European Norms, or ENs, issued by CENELEC. These ENs are not developed by CENELEC but are IEC and CISPR standards redesignated as ENs.

There are three types of EMC Publications:

- **Product EMC Standards**
- **Product Family Standards (including Generic Standards)**
- **Basic EMC Publications**

**Product EMC Standards** relate to a particular type of product, system or installation for which specific conditions must be considered. Product EMC Standards include:

- Resistance Welding equipment
- Measuring Relays and Protection equipment

Product Standards have priority over Product Family and Generic Standards; however, where no Product Standard or Product Family Standard exists for a particular product, the relevant Generic Standard will apply.

**Product Family Standards** apply to products of a particular category such as:

- Household appliances and portable tools
- ITE (Information Technology Equipment)
- Audio, video, audio-visual and entertainment lighting control apparatus for professional use

Product Family Standards have priority over Generic Standards; however, where no Product Family EMC Standard exists for a particular product family, the relevant Generic Standard will apply.

**Generic EMC Standards** are a special type of Product Family Standard which apply to products operating in a particular environment for which no dedicated Product or Product Family Standard exists. They specify a set of essential requirements, test procedures and generalized performance criteria applicable to products or systems operating in this environment.

---

The Generic EMC Standards include: **EN 50082-1**, **EN 50082-2**, **EN 50081-1**, and **EN 50081-2** which cover immunity and emissions testing for commercial, residential and light industrial environments, as well as for industrial environments.

**Basic EMC Publications** may be standards or technical reports which, by definition, are NOT dedicated to specific product families, products, systems or installations. They may concern:

- Terminology
- Descriptions of electromagnetic phenomena
- Specification of compatibility levels (NOT compliance levels)
- General requirements for the limitation of emissions
- Recommendations for test levels for immunity
- Measurement techniques
- Descriptions and classification of the environment

Basic EMC Publications include Basic EMC standards such as the IEC 1000-4-X Series, CISPR 22, CISPR 11, and others.

## **TEST REQUIREMENTS**

The Basic EMC Publications (IEC 1000-4-2, IEC 1000-4-4, etc.) set the waveforms, test environment, and measurement techniques. The **EMCPro** was designed to meet the requirements of these publications.

Test levels are set by the Generic EMC Standards and Product Family Standards. The preprogrammed tests stored in the **EMCPro** are designed to meet the test levels of:

- EN 50082-1      Generic Immunity, Residential, commercial, and light industrial
- EN 50082-2      Generic Immunity, Industrial

## **WRITING A TEST PROCEDURE AND THE TEST REPORT**

Before starting testing, you should create a test procedure. This should identify which European Norms or other test requirements to which you are testing. This should include the test levels, polarities, and number of tests.

Most of the remainder of a test procedure is set by the Basic EMC Publications (IEC 1000-4-2, IEC 1000-4-4, etc.) which define the test setup and environmental limits, in detail.

The test procedure should also describe how the EUT is setup and connected to test equipment and ancillary equipment. If the EUT involves software, a description of which software and software revisions should be included.

---

An important part of both the test procedure and the test report is to establish how the EUT is exercised during the test. Most test procedures recommend that the EUT be operated in "the most sensitive mode". Preliminary testing will usually be required to determine what the most sensitive mode of operation is, which may vary with configuration, software, and operations performed.

Finally, the test procedure should consider what level of disturbances of operation is allowed. Ideally the EUT should operate through testing without disturbance, however there may be disturbances which are considered acceptable, in that they do not result in damage. As an example, the following are four possible levels of system disturbance:

- Normal performance within specification limits;
- Temporary degradation or loss of function which is self-recoverable;
- Temporary degradation or loss of function which requires operator intervention or system reset;
- Degradation or loss of function which is not recoverable due to damage to equipment or components or loss of data.

In no case is it acceptable that the equipment become dangerous or unsafe as a result of testing.

The test report should include the test procedure, the test results, and give an explanation of the results, as required. For acceptance tests, the test report is a required result of testing.

The remainder of this section covers the basic EMC publications in detail; explains the waveforms and testing requirements; and explains how to use the **EMCPro** to meet the requirements of the Basic EMC Publications.

---

The information on IEC requirements -- figures and diagrams, tables and data, and test levels -- are accurate as of the date of printing of this manual. However, the IEC and EN documents are subject to review and change. The information in this manual is intended as a guideline only.

---




# IEC 1000-4-2 -- ESD Testing

## What is Electrostatic Discharge (ESD) Testing?

These tests relate to equipment, systems, sub-systems, and peripherals which may be involved in static electricity discharges (either from persons or adjacent equipment), owing to environmental and installation conditions, such as relative low humidity, use of low-conductivity (artificial fiber) carpets, vinyl garments, etc.

Two different types of tests can be performed with the ESD head - Contact or Air. Contact discharges are tests in which a sharp metal ESD tip physically touches the EUT. This method is regarded as the most repeatable method, and is the only acceptable method for waveform verification and calibration. Air discharges are tests in which a rounded ESD tip is quickly thrust toward the EUT until an ESD event occurs by "leaping" from the ESD tip to the EUT through the air. This method does not yield as repeatable results, but can be used if a contact discharge cannot be performed for some reason or another.

The ESD waveform is characterized by the current in Contact-mode discharge, as defined in the figure and table below:

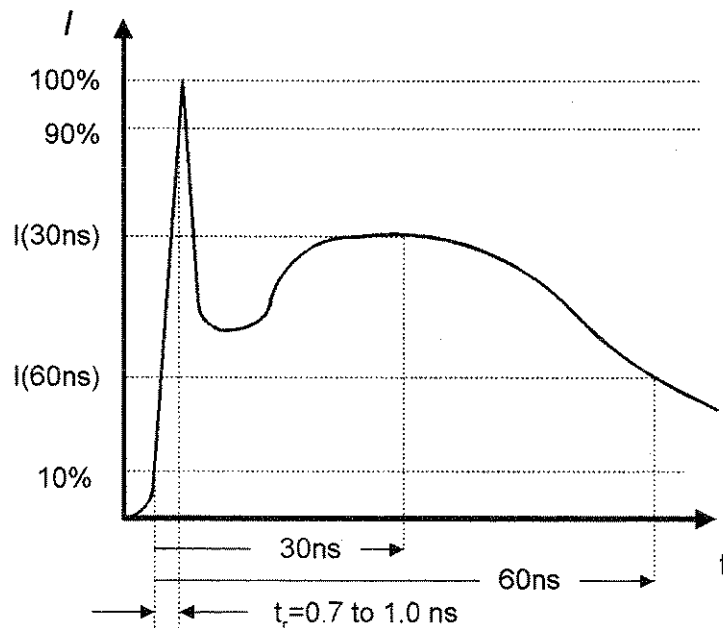

Typical ESD Current Waveform

Level	Set Voltage	Peak Current ( $\pm 10\%$ )	Current ( $\pm 30\%$ ) at 30nS	Current ( $\pm 30\%$ ) at 60nS
1	2 kV	7.5A	4	2
2	4 kV	15 A	8	4
3	6 kV	22.5 A	12	6
4	8 kV	30 A	16	8

## General Guidelines for ESD Testing

Place the air-discharge or contact-mode output tip into the ESD probe output tip receptacle.



The **TPA-2** probe tip is used for air discharge. The rounded tip of this probe prevents pre-discharge corona (which reduces applied voltage) and ensures most consistent results.



The **TPC-3** probe tip is used for contact discharge. The sharp point of this tip will penetrate surface oxidation and -- where necessary -- paint.

Connect the ESD probe to the **EMCPro** using the 8-pin DIN cable. Connect the discharge return cable from the ESD probe to ground (an indicator on the ESD probe will light if the discharge return cable is not connected to the ESD probe). The bargraph indicator on the ESD probe is intended as a rough guide of the actual test voltage, and can serve in many applications as a pulse -- discharge -- indicator. The bargraph display is not calibrated, and can be affected by high humidity; for precise readings of probe tip voltage or periodic calibrations, KeyTek's **DCA-2**, high-voltage divider should be used.

The ESD probe can be operated in manual triggering mode -- normal -- or automatic triggering mode -- tripod. Normal triggering is intended for handheld applications; in normal mode the probe will fire once for each time the probe button is pressed if the repetition is set to one, or fire continuously at 1pps or 20pps while the button is depressed if the repetition is set higher. Tripod triggering mode is intended for tripod operation; in this mode the probe will start triggering when the probe button is pressed and released and operation continues until either: the test ends, the operator ends the test by pressing the STOP -- F1 function -- key, or the probe button is pressed a second time.

For safety, in all modes of operation, the operator must select a program and press run from the **EMCPro** front panel or application software, THEN press the probe button to start the test.

For Contact discharges the **TPC-3** contact tip should physically touch the EUT. For Air discharge the rounded, **TPA-2** tip is thrust toward the EUT at a constant rate until an ESD event occurs by "leaping" from the ESD tip to the EUT through the air. The probe is then pulled back - away from the EUT - in preparation for the next test. Some practice is required to obtain consistent results with air discharge.

Certification testing per European Norms uses 1pps for compliance testing. Use 20 pulses per second mode for quick scans to determine the most sensitive areas; then switch to 1pps for compliance testing. In 20 pps mode the pulse-detection and pulse counting features of the

---

**EMCPro** are disabled -- after the first pulse event, the ESD probe will free-run at 20pps whether or not there is a discharge.


## **ESD Testing Requirements per IEC 1000-4-2**

Testing to IEC 1000-4-2 has the following requirements:


- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 30 % to 60 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)
- A ground reference plane (GRP) is required.
- The EUT shall be positioned at least 1 m from walls and any metallic structures.
- Positioning of power and signal cables shall be representative of good installation practice.
- The EUT shall be connected to the grounding system, representative of good installation practice; no additional earthing connections are allowed.
- The discharge return cable should, where possible, be placed off the ground reference plane, and should not come closer than 0.2 m to other conductive parts of the test setup.
- Vertical Coupling Planes (VCP) and Horizontal Coupling Planes (HCP) may be used for indirect application of the ESD pulse. These planes shall be constructed from the same material and thickness as the ground plane, and should be connected to the ground plane by a cable with two, 470,000 ohm resistors, one resistor at each end of the cable.
- For table-top equipment, a non-conducting table 0.8 m high is placed on the ground plane. A ground plane (HCP) 1.6 m by 0.8 m will be put on the table, and the EUT and any cables shall be placed on an insulating support 0.5mm thick placed on top of the HCP. The HCP shall connect to the ground reference plane with a resistive cable as in the previous paragraph.

IEC 1000-4-2 requires the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is 1 m<sup>2</sup>, the exact size depending on the dimensions of the EUT; the ground plane shall extend beyond the EUT by at least 0.5 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

For Floor-standing EUT the EUT is placed on a non-conducting mat of 0.1 mm minimum thickness placed on the ground plane. ESD testing may be direct -- applied to the EUT -- or indirect -- applied to the ground plane or to a vertical plane bonded to the ground plane.

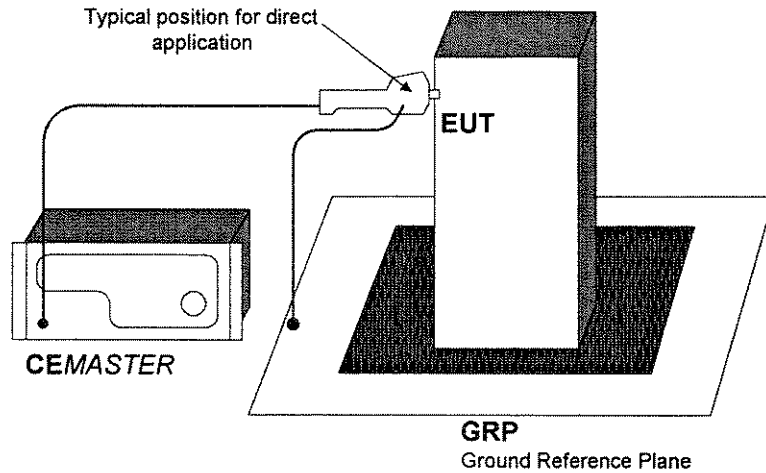

Typical ESD Test Setup for Floor-standing EUT

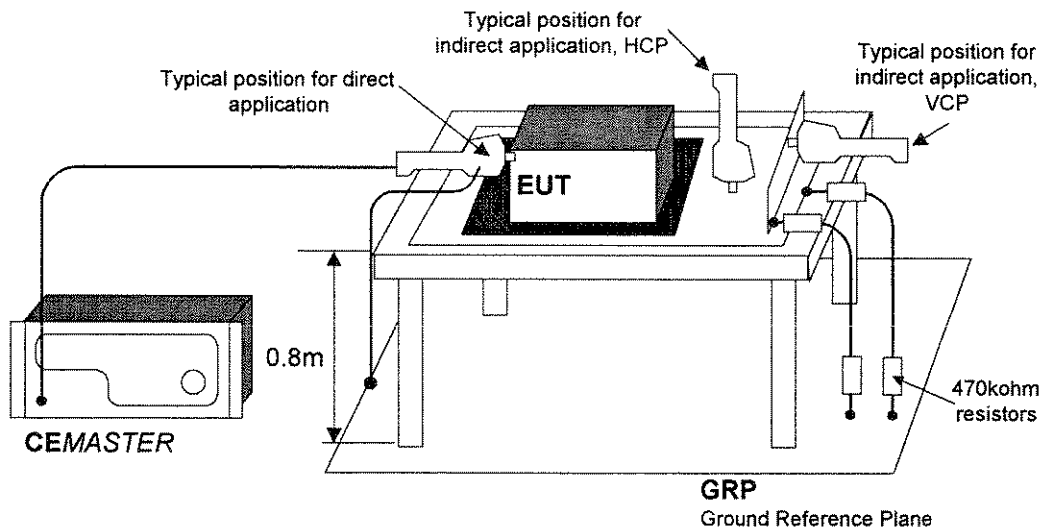

Typical ESD Test Setup for Table-Top EUT

During testing, the EUT is operated in a normal fashion. Compliance testing is typically performed with the EUT continually operating in the most sensitive mode, as determined by preliminary testing.

Pulses are applied to points and surfaces which are accessible to personnel during normal usage. The voltage is increased from the minimum to the selected test level, in order to determine the threshold of failure (if any). The final test level is set by the product specification and the test class. The test is applied with single discharges, at preselected points. At least ten discharges of the most sensitive polarity shall be applied, and a rest interval of at least one second is recommended (or longer, as required to verify continued operation of the EUT).

The **EMCPro** supports 1000-4-2 testing to class 3 in Air-discharge mode and class 2 in contact discharge mode. The following table lists the test capabilities of the ESD hardware:

Class	Peak Voltage kV	
	Contact	Air
1	2	2
2	4	4
3	N/A	8

## User-defined ESD Tests

The user-defined test option allows individual control of all test parameters required for ESD testing; this allows testing at different levels, modes, and repetition rates. The test parameters are:

ESD Test Parameter	Range/Units
<u>Voltage</u>	[-8800...-250, +250...+8800] V; resolution: 5 V
<u>Tip</u>	Air or Contact
<u>Mode</u>	Normal or Tripod
<u>Repetition Rate</u>	[1pps, 20pps]
<u>Number of Pulses</u>	[1 ... 999]

## Preprogrammed IEC Standard ESD Test Sequences

Two preprogrammed test sequences are stored in the **EMCPro** for rapid testing to the IEC standards of IEC 1000-4-2.

There are two tests mandated by the specifications - a 4 kV contact discharge and an 8 kV air discharge. Repetition is set for 1 pps and polarity is set by the user to the most sensitive polarity. The user can select mode -- normal or tripod -- and the number of pulses.

The table below shows these two tests:

Tests	Voltage, kV	Number of Discharges	Repetition, pps
Contact	4	10 positive, 10 negative	1
Air	8	10 positive, 10 negative	1

---

## ESD Waveform Verification

IEC 1000-4-2 requires that the ESD output be verified periodically. Verification requires an ESD target (KeyTek **CTC-3**), a target plane (KeyTek **TP-1**), and an oscilloscope of 1GHz minimum bandwidth. The ESD probe with contact-mode tip is placed on a tripod, the **EMCPro** set to TRIPOD mode, 1pps.

The rise time, peak amplitude, and amplitude at 30 ns and 60 ns should be monitored and recorded and checked against the figure and table at the start of this section.

---

Performing ESD calibration is not trivial. The high-speed oscilloscope is expensive; the extremely fast risetime and high-bandwidth required by specification can require that a dedicated test site be built, with Faraday-shields for the oscilloscope, and EMI damping materials on floors and walls to reduce reflections.

KeyTek offers a calibration service for all equipment, including the ESD probe. Contact factory for details.

---

---

## IEC 1000-4-4 -- EFT Testing

For safety reasons, the precautions taken during EFT testing should be the same as for Surge testing -- read and follow the guidelines of the **Safety Concerns During Surge Testing** section.


It is important that the Equipment Under Test be properly connected -- read and follow the guidelines of the **Test Area Considerations and Site Preparation** section and of the **Special Considerations for EFT Testing** section, as well as the **Testing Requirements per IEC 1000-4-4** section which follows.

---

### What is Electrical Fast Transients (Burst) Testing?

The electrical fast transient test consists of a burst of fast pulses, coupled into power supply, control and signal ports of electrical and electronic equipment. The significant characteristics of the test are very high amplitude, the short rise time, the high repetition rate, and the low energy of the transients.

The test is intended to demonstrate the immunity of electrical and electronic equipment when subjected to types of transient disturbances such as those originating from switching transients (interruption of unsuppressed inductive loads, relay contact bounce, etc.).

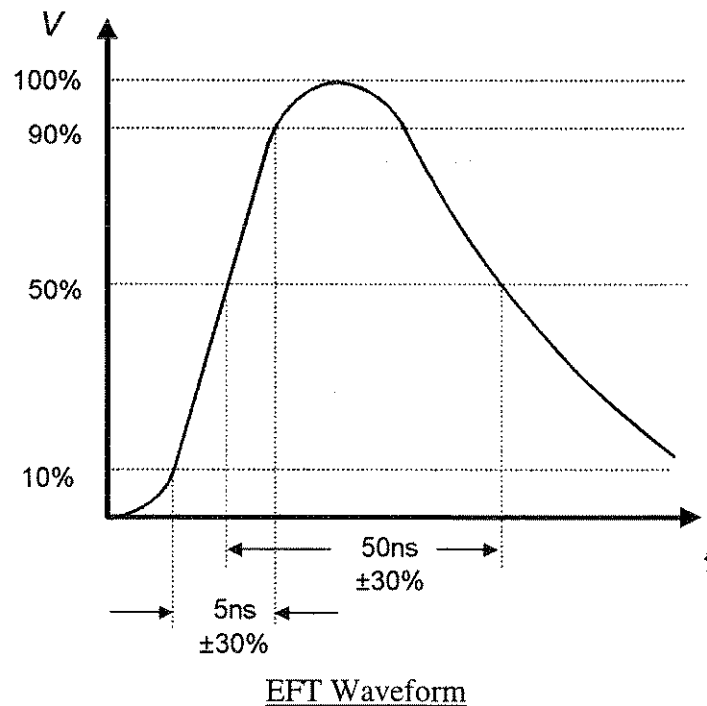

---

## General Guidelines for EFT Testing

The EFT test voltage is referenced to the chassis of the **EMCPro**. The EFT waveform is coupled into the EUT via the AC Mains and the mains coupler built into the **EMCPro**, or via signal lines (or both). An optional Capacitive Cable Clamp is available for coupling to signal lines or to power lines where the **EMCPro** internal coupler cannot be used.

When applied to the EUT Mains, the EFT voltage is applied between ground -- the Ground Reference Plane (GRP) -- and each of the power supply terminals and between the GRP and the protective earth of the EUT.

Power-line -- Mains -- testing is performed by plugging the EUT into the **EMCPro** EUT outlet, establishing the EUT in a normal operating mode, and applying the EFT waveform to, first the line (L1), then neutral (L2), then PE.

Data-line testing starts with the EUT and auxiliary equipment plugged into the **EMCPro** EUT outlet -- to prevent EFT waveforms from contaminating the AC Mains -- and couples the EFT waveform from the CLAMP outlet to a Capacitive Cable Clamp where the waveform is coupled into the signal lines. The Capacitive Cable Clamp should be adjusted to fit snugly about the cables to be tested.

The **EMCPro** contains orientation-sensitive components, and will only perform EFT testing when operated in a horizontal position; for accurate, repeatable results the **EMCPro** should be level, and should be used in a location free from vibration.

## EFT Testing Requirements per IEC 1000-4-4

Testing to IEC 1000-4-4 has the following requirements:


- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 25 % to 75 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)
- A ground reference plane (GRP) is required, and is bonded to building protective earth (PE) ground.
- The EUT shall be positioned at least 0.5 m from walls and any metallic structures.
- The EUT shall be connected to the grounding system, representative of good installation practice; no additional earthing connections are allowed.
- Positioning of power and signal cables shall be representative of good installation practice, EXCEPT:
  - The length of signal and power cables shall be 1 meter or less.
  - If the length of signal or power cable exceeds 1 meter, the excess length shall be gathered into a flat coil with a diameter of 0.4 m and situated at a height of 0.1 m above the GRP.



IEC 1000-4-4 requires the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is  $1 \text{ m}^2$ , the exact size depending on the dimensions of the EUT and **EMCPro**; the ground plane shall extend beyond the EUT and **EMCPro** by at least 0.1 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

The cabinet of the **EMCPro** must be directly tied to the ground reference plane. Provision for a mounting bracket is made on the rear of the **EMCPro** and the bracket and screws are provided.

Grounding Bracket




Rear View


Location of Grounding Bracket

For floor mounted equipment, the EUT shall be placed on the GRP and shall be insulated from the GRP by an insulating support 0.1 meter  $\pm$  0.01 meter thick.

For table-top equipment, the EUT should be placed on a table of height 0.8 meter  $\pm$  0.08 meter above the GRP.

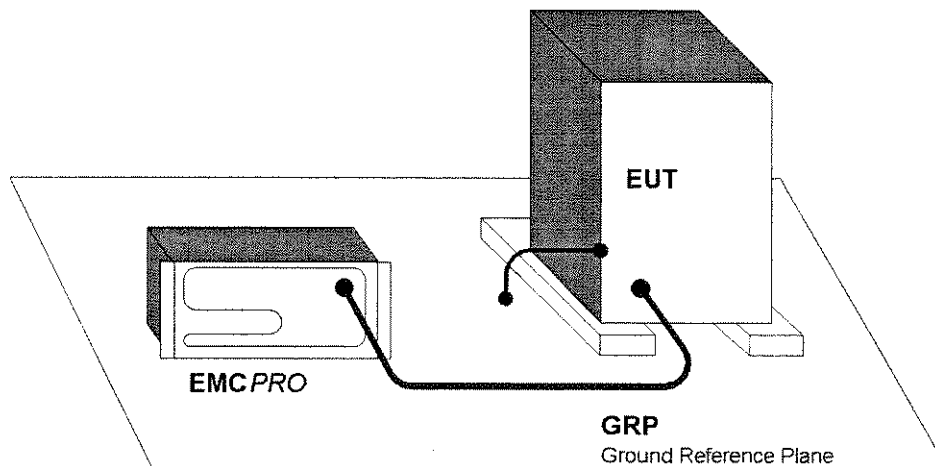


EFT Connection to Equipment Under Test for Floor-standing EUT

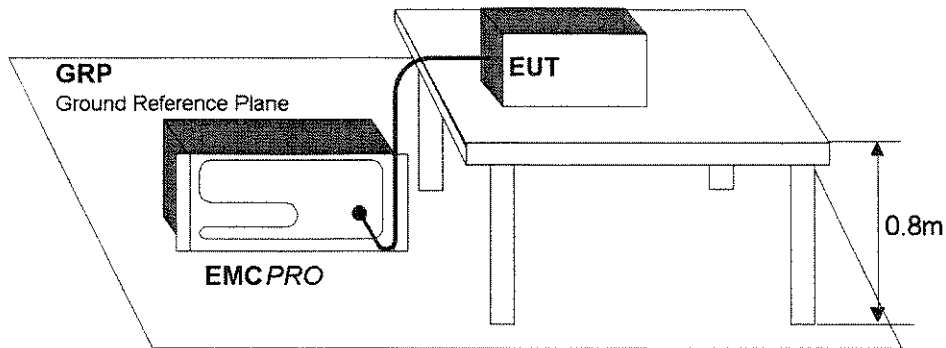

EFT Connection to Equipment Under Test for Table-top EUT

Data and signal cables are tested using the EFT Capacitive Coupling Clamp (CM-CCL). When performing these tests, the EUT and any auxiliary equipment should be powered from the **EMCPro** EUT output, to provide isolation between the test setup and building power mains. The minimum spacing required between the clamp and the equipment in the test area is shown in the figure below (Note: if the Auxiliary equipment is not considered part of the EUT, the separation distance is 5 meters as shown. If the Auxiliary equipment is considered part of the EUT, the separation drops to 1 meter).

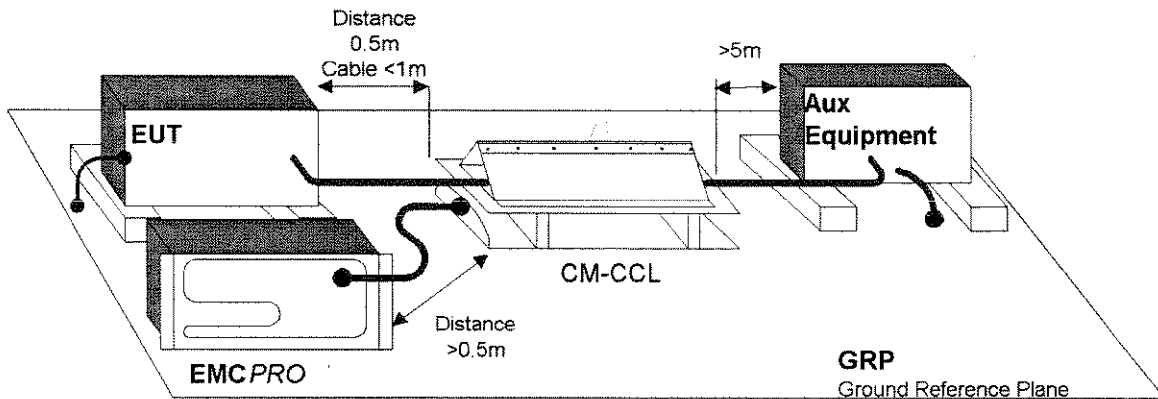

Use of the Capacitive Cable Coupler for EFT Testing

The voltage test levels to be applied vary with the test class, and are listed below:

Test Level	Peak Voltage	Frequency	Peak Voltage	Frequency
Class 1	500V	5kHz	0.25kV	5kHz
Class 2	1.0kV	5kHz	0.5kV	5kHz
Class 3	2.0kV	5kHz	1.0kV	5kHz
Class 4	4.0kV	2.5kHz	2.0kV	5kHz

The level used in testing depends on the European Norm (EN) chosen to test against. As example, EN50082-1 (for Residential, commercial, and light industry) specifies a test level of 1000 volts. The EFT voltage is applied for one minute, for each test.

## User Defined EFT Test

The user-defined test option allows individual control of all test parameters required in EFT testing; this allows testing at different levels, modes, and repetition rates.

On being triggered by pressing the “start” key, a user defined test produces a series of output events with the parameters defined below:

Parameter	Range	Resolution	Accuracy
Voltage	-250V ... -4400V, 250V ... 4400V	1V	+/- 10%
Burst Frequency	2.5 ... 100kHz in 0.5kHz steps	0.5kHz	+/- 20%
Output Coupling	Clamp, Mains [Mains modes, L1, L2, PE, L1&L2, L2&PE, L1&PE, or L1&L2&PE All outputs with respect to Groundplane]		
Test Duration	1...999 seconds	1 second	

## Preprogrammed EFT Test Sequences

Three preprogrammed test sequences are stored in the **EMCPro** for rapid testing to the IEC standards. These test sequences are designed to satisfy the requirements of EN50082-1 and EN50082-2.

Test Sequence	Peak Voltage	Frequency	Port	Coupling Mode Mains only	Number of Bursts
Class 1	500V	5kHz	Mains or Clamp	PE to groundplane.	200 (1 minute) per polarity
Class 2	1.0kV	5kHz	Mains or Clamp	L1, L2, and PE in sequence	200 (1 minute) per polarity and coupling mode
Class 3	2.0kV	5kHz	Mains or Clamp	L1, L2, and PE in sequence	200 (1 minute) per polarity and coupling mode
Class 4	4.0kV	2.5kHz	Mains or Clamp	L1, L2, and PE in sequence	200 (1 minute) per polarity and coupling mode

All tests are run twice: once in each polarity.


---

## EFT Waveform Verification

IEC 1000-4-4 requires that the EFT output be verified periodically. For verification, the output of the generator is connected to an oscilloscope through a 50-ohm, high-voltage coaxial attenuator. The rise time, duration, and repetition rate of the impulses within one burst should be monitored and recorded. The amplitude into 50 ohms is one-half of the programmed voltage,  $\pm 10\%$ .

The bandwidth of oscilloscope and attenuator must exceed 400MHz. For digital oscilloscopes a sampling rate exceeding 1GSa/s is recommended. The attenuator must have a voltage rating of 1250V minimum.

The test setup shown below is usable for Waveform Verification. The BARTH Model 2237HFNFP attenuator<sup>4</sup> has sufficient voltage and power rating to connect directly to the **EMCPro** output. The Tektronix<sup>5</sup> attenuators drop the voltage to within the range of typical oscilloscope inputs. The circuit below provides a total attenuation of 1000:1.

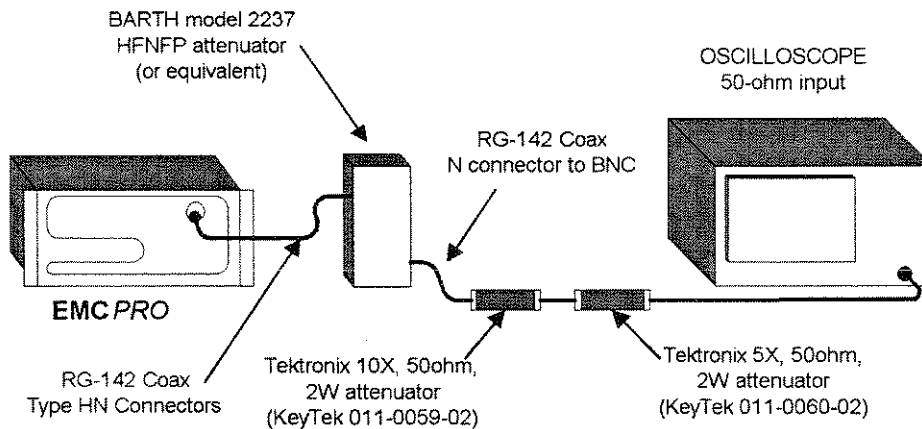

### Recommended Test Setup for Waveform Verification



#### CAUTION

The circuit above is for measurement of the EFT waveform at the HN-coax connector; this circuit is not rated for use across the AC Mains outlet.

**Connecting this circuit across the AC Mains with Mains voltage present will result in damage of the attenuator.**

If measuring EFT waveform at the AC Mains outlet: Check that the EUT switch is off and no AC is applied to the EUT Mains Inlet before connecting the attenuator; make the measurement and remove the attenuator immediately.

---

<sup>4</sup> Barth Electronics, Inc., 1300 Wyoming St., Boulder City, NV 89005 USA

<sup>5</sup> Tektronix, Inc., P.O. Box 1000, Wilsonville, OR 97070-1000 USA

---

# SURGE Testing

---

Surge testing is hazardous -- read and follow the guidelines of the **Safety Concerns During Surge Testing** section.

It is important that the Equipment Under Test be properly connected -- read and follow the guidelines of the **Test Area Considerations and Site Preparation** section and of the **Special Considerations for Surge Testing** section.

---


## What is Surge Testing?

Surge testing is the application of unidirectional surges to the Equipment Under Test to model those caused in the real world by overvoltages from switching and lightning transients.


Surges occur on the AC power mains as a result of switching operations in the power grid and from nearby lightning strikes, either directly to the power distribution system or to nearby ground. Radiated coupling of surges into I/O lines can also occur.

Electronic products are tested for Surge immunity to insure their continued reliable operation if subjected to realistic levels of surge voltages.

The waveform used for IEC testing of the AC Mains and I/O lines is the 1.2/50  $\mu$ s open circuit voltage (8/20  $\mu$ s short circuit current) combination wave. This waveform is separately characterized by the open circuit voltage and short circuit current.

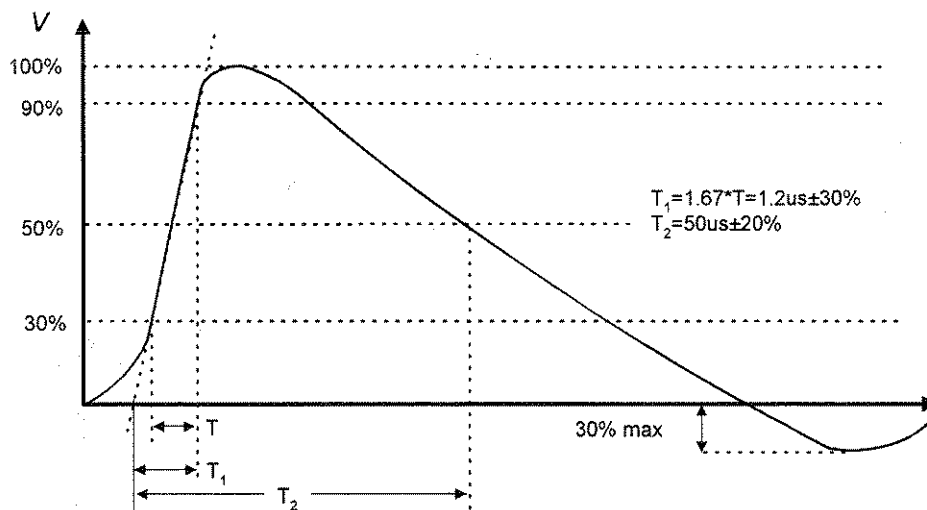


Combination Wave-Open-Circuit Surge Voltage

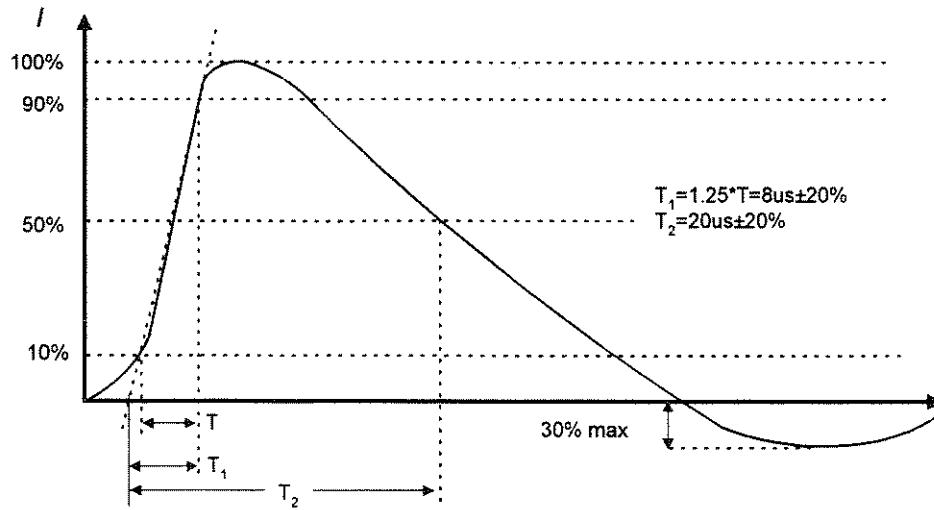


Combination Wave-Short-Circuit Surge Current

The waveform for IEC testing of communication lines (I/O lines) and telecommunication lines is the 10/700us waveform; the open circuit voltage and short circuit current for this waveform are defined in the figures below. The current waveform has a peak current of 400A at 6000V programmed voltage. The current waveform is defined with 40 ohms series impedance, requiring the addition of 25 ohms outside of **EMCPro**.

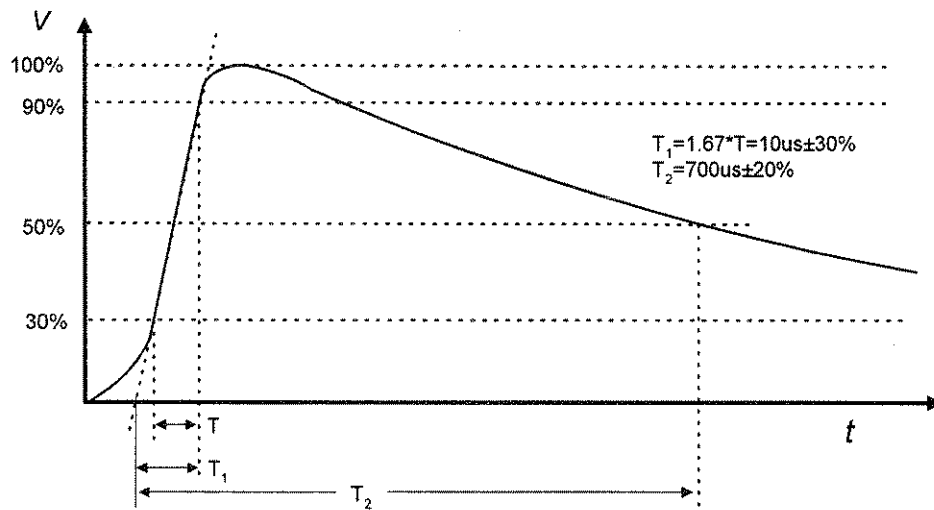


10/700us Voltage Waveform per IEC 1000-4-5 and CCITT

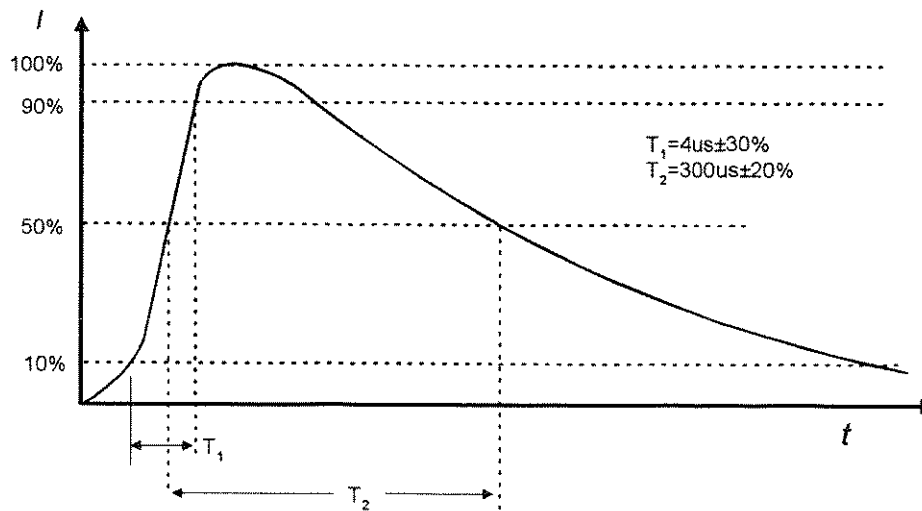

10/700us Current Waveform per IEC 1000-4-5 and CCITT

In the **EMCPro** the 10/700us Waveform is an option; this waveform is only available with the purchase of the **PRO-SURGE+TELECOM** or **PRO-TELECOM** option.

As an alternative, a 100kHz Ringwave can be substituted for the 10x700us Waveform. Available as option, **PRO-SURGE+RING** or **PRO-RING**, the Combination Wave allows testing of power mains per the IEC standards, and the 100kHz Ringwave and Combination Waveform allows testing to the requirements of IEC 1000-4-12 and ANSI / IEEE C62.41-1991. The Ringwave risetime is 0.5 vs (10-90%). The Ringwave has two waveforms available, described by their peak, short-circuit current: a 200A peak current Ringwave at 6000V and a 500A peak current Ringwave at 6000V.

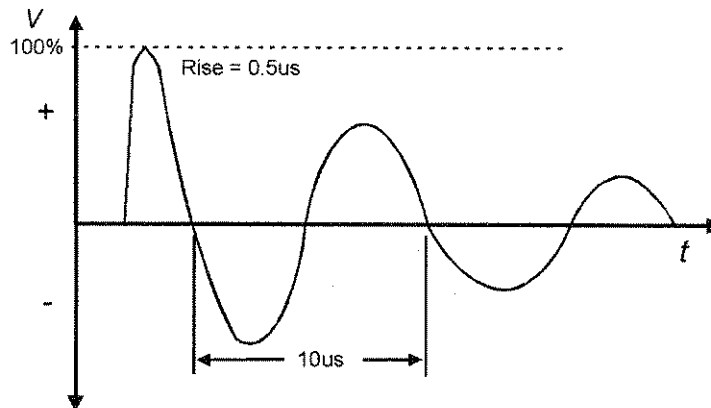

100kHz Ringwave Waveform per IEC 1000-4-12 and ANSI / IEEE C62.41-1991

## General Guidelines for Surge Testing

Surge testing is very useful to determine if breakdown of components will occur when subjected to a high-voltage impulse. Surge testing can be performed on AC or DC power Mains, communications lines, and components.

---

The **EMCPro** includes a built-in coupler which can place combination-wave or Ringwave surges on AC or DC Mains for application to the EUT. The 10/700  $\mu$ s waveform is not available through the coupler - as a Telecommunications waveform, it is only available from the front panel. The angle of application onto the AC Mains waveform can be precisely controlled; application at 90° and 270° cause the surge to add to the peak line voltage for worst-case voltage; application at other angles can be used to find sensitive components -- such as diodes, SCRs, or solid-state switches -- which are most sensitive at the time they turn on or off.

The **EMCPro** also has front panel, safety socket connections to apply surges to the magnetic field test coil (**CM-HCOIL**) or for component testing. The **CM-I/OCD, and PRO-TELECOM** optional accessories provide convenient coupling of surges onto data and telecom lines.

When surging a DC Mains or the EUT with no mains applied, the Line Coupling Phase Angle selection must be set to 'RND' -- random -- otherwise the test would be unable to synchronize to a DC mains and would not run.

The **EMCPro** contains orientation-sensitive components, and will only perform Surge testing when operated in a horizontal position; for accurate, repeatable results, the **EMCPro** should be level, and should be used in a location free from vibration.

Probing the EUT during Surge testing should be attempted only by experienced test engineers. When connecting probes to the EUT, follow these guidelines:


- Use balanced, differential, high-voltage probes rated for the surge voltage (such as the KeyTek PK1001D probe set). Most oscilloscope probes are rated for 600Vac or less and should NOT be used in Surge testing.
- Current should be measured with a non-contact, high-bandwidth current transformer (a Pearson<sup>6</sup> model 110 current transformer, or equivalent).
- **Do not connect probe grounds to the EUT!** This will create a path for Surge and fault currents which can endanger the operator and test equipment.
- **Do not defeat protective grounding or earthing of the oscilloscope or other test instrument.**
- If connecting a voltmeter or other high-impedance test equipment to the EUT, carefully check the common-mode voltage rating of the equipment. This is the voltage rating of both probes above the instrument ground. Surge testing will typically exceed the common-mode voltage rating of most Mains-powered equipment, and can exceed the rating of battery-powered

---

<sup>6</sup> Pearson Electronics, Inc., 1860 Embarcadero Rd., Palo Alto, CA 94303 USA



equipment. Use of an instrument above its common-mode voltage rating may result in improper operation or damage.

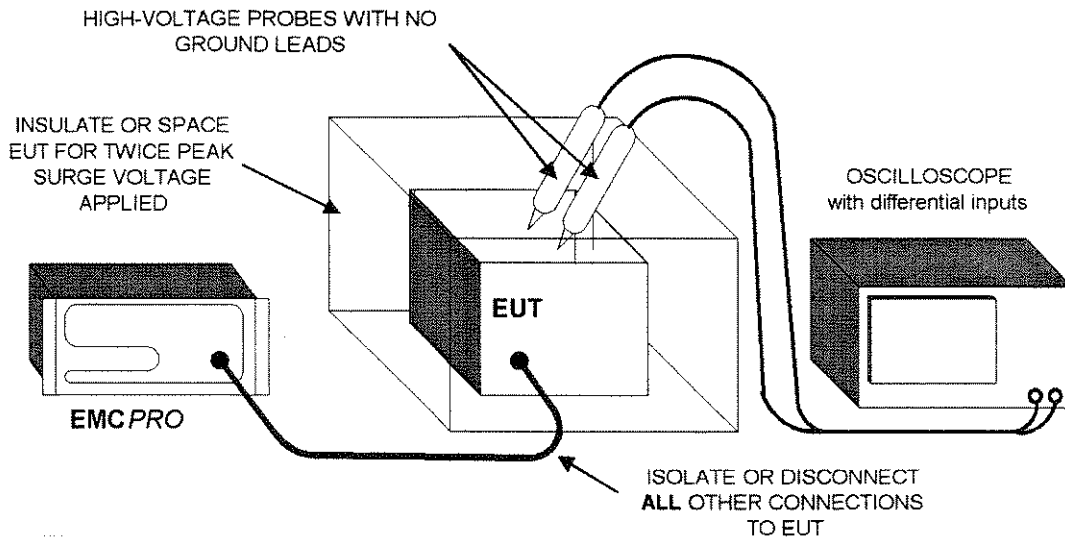

Connection of Probes to the EUT during Surge Testing

---

## Surge Testing Requirements per IEC 1000-4-5

The Basic EMC Standards for Surge define the methods of generating consistently reproducible surge voltages for test purposes. They specify generator and coupler/decoupler design and performance in sufficient detail to produce correlatable results between test sites. These are issues which are controlled by the design of the **EMCPro** and need not be considered by the operator or user.

While the Basic EMC Standard specifies how to perform Surge testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria. IEC 1000-4-5 also includes a climatic specification, as follows:

- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 10 % to 75 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)Note that other values may be specified in the test specification. The EUT should be operated within its intended climatic conditions.

The test level, polarity, and source impedance are set by the European Norms (EN), as a function of use and exposure class (See the Class Definition Table and Test Levels Table, below). The **EMCPro** is capable of testing to Classes 0, 1, 2, 3, 4, and 5 test levels.

The general test requirements, per IEC 1000-4-5 are as follows:

<b>Output polarity</b>	Both positive and negative
<b>Output (source) impedance</b>	For power supply (AC or DC), line to line surges: 2 $\Omega$ For power supply (AC or DC), line to earth surges: 12 $\Omega$ For direct coupling to communication lines: 40 $\Omega$ (2 or 12 $\Omega$ selected from <b>EMCPro</b> , and additional, external resistance added)
<b>Number of tests</b>	At least five positive and five negative tests at each test level
<b>Repetition rate</b>	Maximum: 1 surge per minute
<b>Mains Synchronization</b>	0° or 180°, 90°, and 270°

**Class definitions**

Class 0	Well-protected electrical environment, often within a special room.
Class 1	Partly protected electrical environment.
Class 2	Electrical environment where the cables are well separated, even at short runs.
Class 3	Electrical environment where cables run in parallel.
Class 4	Electrical environment where the interconnections are running as outdoor cables along with power cables, and cables are used for both electronic and electric circuits.
Class 5	Electrical environment for electronic equipment connected to telecommunication cables and overhead power lines in a non-densely populated area.
Class x	Special conditions specified in the product specification.

**Voltage Test Levels vs. Class, Combination wave**

Class	Test levels (kV)							
	Power supply Coupling Mode (Combination)		Unbalanced datalines, LDB Coupling mode (Combination)		Balanced datalines Coupling mode (Telecom)		SDB, DB <sup>1)</sup> Coupling mode (Combination)	
	Line to line	Line to earth	Line to line	Line to earth	Line to line	Line to earth	Line to line	Line to earth
0	NA	NA	NA	NA	NA	NA	NA	NA
1	NA	0.5	NA	0.5	NA	0.5	NA	NA
2	0.5	1.0	0.5	1.0	NA	1.0	NA	0.5
3	1.0	2.0	1.0	2.0 <sup>3)</sup>	NA	2.0 <sup>3)</sup>	NA	NA
4	2.0	4.0 <sup>3)</sup>	2.0	4.0 <sup>3)</sup>	NA	2.0 <sup>3)</sup>	NA	NA
5	2) <sup>2)</sup>	2) <sup>2)</sup>	2.0	4.0 <sup>3)</sup>	NA	4.0 <sup>3)</sup>	NA	NA
x								

1) Limited distance, special configuration, special layout, 10 m to max. 30 m: no test is advised at interconnection cables up to 10 m, only class 2 is applicable.

2) Depends on the class of the local power supply system.

3) Normally tested with primary protection.

Explanation:

DB	=	data bus (data line)	SDB	=	short-distance bus
LDB	=	long-distance bus	NA	=	not applicable

## User Defined Surge Tests

The User Defined menu allows individual control of all test parameters required in surge testing; this allows testing at different levels, modes, and repetition rates.

A User defined Surge Test is controlled by a set of test parameters and results in a surge event, or number of surge events, whose parameters are defined in the tables below.

### User Defined Surge Test -- 1.2/50us Combination Wave

Surge Test Parameter	Range/Units
<u>Waveform</u>	Auto, 2, 12 $\Omega$ Output Impedance (source impedance) For Waveform = "Auto": If the Output is MAINS and the Line Coupling is PE, then the Output Impedance is 12 $\Omega$ ; otherwise the Output Impedance is 2 $\Omega$ .
<u>Surge Voltage</u>	[-6600..+6600] V; resolution: 1 V
<u>Output</u>	Direct (safety sockets), MAINS (EUT output receptacle)
<u>Line Coupling</u>	For <u>Output</u> = Direct : [N/A] For <u>Output</u> = MAINS: ( <sup>Surge HIGH</sup> / <sub>Surge LOW</sub> ) = [ <sup>L1</sup> / <sub>L2</sub> , <sup>L1</sup> / <sub>PE</sub> , <sup>L2</sup> / <sub>PE</sub> , ( <sup>L1 and L2</sup> )/ <sub>PE</sub> ]
<u>Line Coupling Phase Angle</u>	For <u>Output</u> = Direct : [not applicable] For <u>Output</u> = MAINS: [Random, 0..360 °]; resolution: 1° Random is required when surging a DC Mains, or when surging the EUT outlet with no EUT power applied.
<u>Interval Between Tests</u>	(15..999) s; resolution: 1 s If a number is entered which is less than the minimum time required to charge the circuit to the required <u>Surge Voltage</u> , the time will be replaced with the minimum time.
<u>Number of Tests</u>	[1..999] When the operator presses the START key, the system will execute the specified number of Charge and Surge cycles; the surge will occur automatically every <u>Interval Between Tests</u> , preceded by an audible warning.

## User Defined Surge Test -- 10/700us Wave

Surge Test Parameter	Range/Units
<u>Surge Voltage</u>	[-6600..+6600] V; resolution: 1 V
<u>Interval Between Tests</u>	(15..999) s; resolution: 1 s If a number is entered which is less than the minimum time required to charge the circuit to the required <u>Surge Voltage</u> , the time will be replaced with the minimum time.
<u>Number of Tests</u>	[1..999] When the operator presses the START key, the system will execute the specified number of Charge and Surge cycles; the surge will occur automatically every <u>Interval Between Tests</u> , preceded by an audible warning.

## User Defined Surge Test – 100kHz Ringwave

Surge Test Parameter	Range/Units
<u>Waveform</u>	200A, 500A
<u>Surge Voltage</u>	[-6600..-250, +250..+6600] V; resolution: 1 V
<u>Output</u>	Direct (safety sockets), MAINS (EUT output receptacle)
<u>Line Coupling</u>	For <u>Output</u> = Direct : [N/A] For <u>Output</u> = MAINS: $(\text{Surge HIGH}/\text{Surge LOW}) = [L^1/L^2, L^1/PE, L^2/PE, (L^1 \text{ and } L^2)/PE]$
<u>Line Coupling Phase Angle</u>	For <u>Output</u> = Direct : [not applicable] For <u>Output</u> = MAINS: [Random, 0..360 °]; resolution: 1° Random is required when surging a DC Mains, or when surging the EUT outlet with no EUT power applied.
<u>Interval Between Tests</u>	(15..999) s; resolution: 1 s If a number is entered which is less than the minimum time required to charge the circuit to the required <u>Surge Voltage</u> , the time will be replaced with the minimum time.
<u>Number of Tests</u>	[1..999] When the operator presses the START key, the system will execute the specified number of Charge and Surge cycles; the surge will occur automatically every <u>Interval Between Tests</u> , preceded by an audible warning.

---

## Preprogrammed IEC Standard Surge Test Sequences

Each of the preprogrammed tests is a set of sequentially executed tests where most parameter values are predefined. Preprogrammed tests are based on the IEC Installation Class definitions.

“Fast” test sequences perform tests to one and only one Class level, while “Full” test sequences follow the directions of IEC 1000-4-5, testing to a Class test level and all Classes below that level. A “Full” test sequence is required to certify equipment. A “Fast” test sequence allows quickly tracking down problems; e.g. if a unit always passes Class 1 only to fail Class 2, the Fast test can test only the Class 2 level.

After selecting a preprogrammed test you have the options of selecting Line Coupling, and Interval between tests.

To meet the specifications of IEC 1000-4-5 the Interval between tests should be 60 seconds (the default) or greater. Use a larger interval, if needed, to verify operation of the EUT between pulses. While you can use a shorter interval to speed pre-qualification testing, note that the surge event can cause stress to the EUT; applying surges at too fast a rate may be overly stressful and could result in damage to the EUT. The time to complete column in the following table assumes the default Interval between tests is used.

When Line Coupling is set to MAINS, the **EMCPro** cycles through each line coupling mode: L1-to-L2, L1-to-PE , and L2-to-PE.

When surging a DC Mains or the EUT with no mains applied, the Line Coupling Phase Angle selection must be set to ‘RND’ --random -- otherwise the test would be unable to synchronize to a DC mains and would not run.

## Preprogrammed Test Sequences -- 1.2/50us Combination Wave

Test	Surge Voltage**		Time to Complete (hrs:min)	
	L1-to-L2	L1-to-PE & L2-to-PE	Direct Coupling	Mains Coupling
Class 2 Fast	500	1000	00:10	01:30
Class 3 Fast	1000	2000	00:10	01:30
Class 4 Fast	2000	4000	00:10	01:30
Class 1 Full	NT	500	00:10	01:30
Class 2 Full				
Step 1	NT	500	00:30	04:30
Step 2	500	1000		
Class 3 Full				
Step 1	NT	500	00:30	04:30
Step 2	500	1000		
Step 3	1000	2000		
Class 4 Full				
Step 1	500	1000	00:30	04:30
Step 2	1000	2000		
Step 3	2000	4000		

\* not required for Class 1 test (see Class 1 Full test), but included for convenience to aid in preliminary execution of Class 2 and Class 3 tests

\*\* for Line Coupling = "N/A" (no line coupling), the Surge Voltage will be the same as for line to earth coupling (<sup>L1</sup>/PE and <sup>L2</sup>/PE)

Explanation:    NT       =       no test

## Preprogrammed Test Sequences -- 10/700us Wave

Test	Surge Voltage
Level 1 Fast	500
Level 2 Fast	1000
Level 3 Fast	2000
Level 4 Fast	4000

## Preprogrammed Test Sequences -- Ringwave

Test	Voltage
2kV 200A ANSI	2000
4kV 200A ANSI	4000
6kV 200A ANSI	6000
2kV 500A ANSI	2000
4kV 500A ANSI	4000
6kV 500A ANSI	6000
Lev1 200A IEC	500/250
Lev2 200A IEC	1000/500
Lev3 200A IEC	2000/1000
Lev4 200A IEC	4000/2000
Lev1 500A IEC	500/250
Lev2 500A IEC	1000/500
Lev3 500A IEC	2000/1000
Lev4 500A IEC	4000/2000

Ringwave tests perform 5 tests at each: of 2 polarities; of 4 coupling modes (L1-PE, L2-PE, L1, L2-PE, L1-L2) , at line synchs of 0°, 90°, and 270°. IEC test levels are the first figure for tests to PE, and the second for L1-L2



---

## Surge Waveform Verification

IEC 1000-4-5 requires that the simulator output be verified periodically. High voltage differential surge probes are required for verifying the open-circuit voltage, and a suitable current transformer is required for verification of the short-circuit current. A digital or storage oscilloscope with 100MHz bandwidth is sufficient for measuring the surge voltage and current waveforms and peaks.

The probes are connected across the lines to be verified (e.g. L1 and L2), the generator is programmed to apply a pulse to these lines, and the signal is captured by the oscilloscope. The peak value, rise, and duration is measured and calculated and compared to the waveforms at the beginning of this section. The tolerance for peak voltage and current is  $\pm 10\%$ .

When measuring current at the EUT outlet, the EUT outlet must be switched off and the EUT Mains power cord should be removed from the inlet for safety. When measuring voltage across the EUT output, the AC Mains should be switched off and the line synchronization set to RANDOM; this simplifies measurements, as the Surge Voltage waveform will not be superimposed on the Mains waveform.

---

## IEC 1000-4-8

# POWER-FREQUENCY MAGNETIC FIELD Testing

### What is Power Frequency Magnetic Field (PFMF) Testing?

Electronic products are often subjected to magnetic fields at AC mains frequencies. These fields are frequently produced in the vicinity of power transformers and can cause problems with CRT's, Hall effect sensors, and other electronic products having a sensitivity to magnetic fields.

Electronic Products are tested for immunity to power frequency magnetic fields to insure their continued reliable operation when placed in service.

### General Guidelines for PFMF Testing

The test magnetic field is applied by the immersion method to the EUT; in this method the EUT is placed in the center of an induction coil.

- The coil is connected to the **HCOIL** - 1.2/50us - Ring Output terminals on the **EMCPro** - top right on the front panel

The induction coil is characterized by a test volume, and an Induction Coil Factor; the coil factor is the ratio between the magnetic field strength generated by an induction coil and the current value required to obtain that field strength. For a standard coil, the coil factor is determined by the manufacturer of the coil, and can be verified by laboratory measurements before carrying out the tests.

The size and shape of the induction coil may vary, but one standard coil is the one-meter square coil available from KeyTek as **CM-HCOIL**. This coil is capable of providing a constant field-strength over a volume of 0.6 by 0.6 by 0.5 meter; for EUT larger than this, a larger coil will be required. The Coil Factor for this coil is 0.87.

Since the Equipment Under Test may show sensitivity to the direction of magnetic field, the coil or EUT is typically rotated to apply the field in three orthogonal directions.

The unit of magnetic field measurement is A/m. In free-space, 1 A/m is equivalent to 1.26 micro-Teslas or 0.0126 Gauss.


The **EMCPro** operates as a current-controlled device -- it generates a sinusoidal output current. The maximum Magnetic Field Strength available in a test is dependent upon the Induction Coil Factor of the Induction Coil, as the Magnetic Field Strength is the product of the Surge Current and the Induction Coil Factor.

The **EMCPro** can source 5 amperes; this is sufficient to drive a coil with coil-factor of 0.8. to 4 A/m. With lesser coil factors, the current will increase, and this may cause distortion of the

---

sinusoidal current. When the programmed magnetic field strength, divided by the coil factor, exceeds 5 amperes, the current should be checked for indications of distortion.

The **EMCPro** is calibrated with the KeyTek supplied coil and cable - use of other coils or cables may not be calibrated and may require measurements of the current.

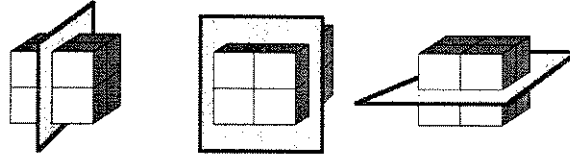

Example of the three Orthogonal Axes for Magnetic Field Testing

## **PFMF Testing Requirements per IEC 1000-4-8**

Testing to IEC 1000-4-8 has the following requirements:

- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 25 % to 75 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)
- A ground reference plane (GRP) is required, and is tied to building Protective Earth (PE) ground.
- The EUT shall be connected to the grounding system, representative of good installation practice.
- Positioning of power and signal cables shall be representative of good installation practice.
- A back-filter, to prevent possible interference with other equipment, is optional in IEC 1000-4-8, although required in the Pulsed Magnetic Field testing. The **EMCPro** EUT output may be used as a mains back-filter if desired.

IEC 1000-4-8 requires the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is 1 m<sup>2</sup>, the exact size depending on the dimensions of the EUT; the ground plane shall extend beyond the EUT by at least 0.5 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

The EUT is placed on the ground reference plane, on an insulating support 0.1 meter thick. The EUT is operated normally and the magnetic field is applied. The coil is rotated twice and the test is repeated.

IEC 1000-4-8 requires that one terminal of the test generator be attached to the ground reference plane; the **EMCPro** does this internally. You should not make an external connection between coil and ground reference plane.

---

## User Defined Power Frequency Magnetic Field Test

The User Defined menu allows individual control of all test parameters required in Power Frequency Magnetic Field Immunity Testing; this allows testing at different levels, frequencies, and durations.

A User-defined test is controlled by the parameters in the table below:

Test Parameter	Range/Units
<u>Coil Factor</u>	0.65...1
<u>Field Strength</u>	0...4 A/m, in steps of 0.25 A/m
<u>Line Frequency</u>	50Hz, 60Hz
<u>Duration</u>	1...9999 seconds

## Preprogrammed IEC Standard PFMF Immunity Test Sequences

There are no preprogrammed tests for Power Frequency Magnetic Field Immunity Testing.

### PFMF Waveform Verification

IEC 1000-4-8 requires that the simulator output be verified periodically. This is to ensure that the EUT is being tested at the proper test level. Waveform Verification takes place with the same setup as for EUT testing, but with the EUT removed.

Verification requires a magnetic-field strength meter. KeyTek offers a magnetic-field strength meter, **CM-HMON**, for use in Verification.

The **EMCPro** is set for the desired field strength. The magnetic-field strength meter is placed in the center of the coil and oriented to achieve a maximum reading. The reading of the field meter is compared to the desired field-strength, and the coil factor adjusted accordingly: lower if the measured field strength is too low, higher if the measured field strength is too high. The measurement and adjustment may be repeated until the measured field strength is within acceptable tolerances of the desired field strength.

---

## IEC 1000-4-9

# PULSED MAGNETIC FIELD Testing

### What is PULSED MAGNETIC FIELD (PMF) Testing?

Pulse Magnetic fields are produced as a result of a large current impulse through a conductor. An example is lightning current flowing through a grounding conductor at a power sub-station. Pulse magnetic fields can also occur in heavy industrial areas where very large currents are switched in a manufacturing process.

- The coil is connected to the **HCOIL** - 1.2/50us – Ring Output terminals on the **EMCPro** – top right on the front panel

Electronic products are tested for immunity to pulse magnetic fields to insure their continued reliable operation when placed in service in a very harsh environment.

### General Guidelines for PMF Testing

The test magnetic field is applied by the immersion method to the EUT; in this method the EUT is placed in the center of an induction coil.

A test volume and an Induction Coil Factor characterize the induction coil; the coil factor is the ratio between the magnetic field strength generated by an induction coil and the current value required to obtain that field strength. For standard dimension coil, the coil factor is determined by the manufacturer of the coil, and can be verified by laboratory measurements before carrying out the tests.

The **EMCPro** operates as a current-controlled device -- it outputs a current pulse. The maximum Magnetic Field Strength available in a test is dependent upon the Induction Coil Factor of the Induction Coil, as the Magnetic Field Strength is the product of the Surge Current and the Induction Coil Factor.


The size and shape of the induction coil may vary, but one standard coil is the one-meter square coil available from KeyTek as **CM-HCOIL**. This coil is capable of providing a constant field-strength over a volume of 0.6 by 0.6 by 0.5 meter; for EUT larger than this, a larger coil will be required. The Coil Factor for this coil is 0.87.

Since the Equipment Under Test may show sensitivity to the direction of magnetic field, the coil or EUT is typically rotated to apply the field in three orthogonal directions.

The unit of magnetic field measurement is A/m. In free-space, 1 A/m is equivalent to 1.26 micro-Teslas or 0.0126 Gauss.

---

The **EMCPro** contains orientation-sensitive components, and will only perform Surge testing when operated in a horizontal position; for accurate, repeatable results the **EMCPro** should be level, and should be used in a location free from vibration.

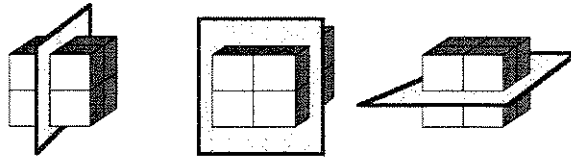

Example of the three Orthogonal Axes for Magnetic Field Testing

## **PMF Testing Requirements per IEC 1000-4-9**

Testing to IEC 1000-4-9 has the following requirements:

- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 25 % to 75 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)
- A ground reference plane (GRP) is required, and is bonded to the building Protective Earth (PE) ground.
- The EUT shall be connected to the grounding system, representative of good installation practice.
- The coil and EUT shall be positioned at least 1 meter from walls and metallic objects.
- A back-filter is required to prevent possible interference with other equipment. The **EMCPro** EUT output may be used as a mains back-filter, or a Line-impedance-stabilization-network (LISN) may be substituted. The user may have to provide additional backfilters for signal and communication lines (if any).
- Positioning of power and signal cables shall be representative of good installation practice, with the following notes:
  - Communication lines shall be maintained at a height of 0.1 meter above the GRP.
  - Backfilters on communication lines -- if used -- shall be at least one meter from the EUT.

IEC 1000-4-9 requires the use of a ground plane which must be bonded to building Protective Earth (PE) ground. The minimum size of the ground plane is 1 m<sup>2</sup>, the exact size depending on the dimensions of the EUT; the ground plane shall extend beyond the EUT by at least 0.5 m on all sides. The ground plane shall be sheet copper or aluminum of 0.25 mm minimum thickness, or 0.65 mm minimum thickness if another metal is used.

The EUT is placed on the ground reference plane, on an insulating support 0.1 meter thick. The EUT cabinet is connected to the ground plane via the EUT earth terminal (if any). The EUT is operated in a normal fashion and pulses are applied. The coil is rotated twice and the test is repeated.

IEC 1000-4-9 requires that one terminal of the test generator be attached to the ground reference plane; the **EMCPro** does this internally. You should not make an external connection between coil and ground reference plane.

## PMF User Defined Pulsed Magnetic Field Immunity Test

The User Defined menu allows individual control of all test parameters required in Pulsed Magnetic Field Immunity Testing; this allows testing at different levels, number of pulses, and time between tests.

A User-defined test is controlled by the parameters in the table below:

PMF Test Parameter	Range/Units
<u>Coil Factor</u>	[0.5..1.0]; resolution: 0.01
<u>Magnetic Field Strength</u>	[-1100..-50,..+1100] The <u>Magnetic Field Strength</u> is dependent upon the <u>Coil Factor</u> selected, as <u>Magnetic Field Strength</u> is the product of the <u>Surge Current</u> and the <u>Coil Factor</u> . The above range assumes a coil factor of 0.87; the actual <u>Magnetic Field Strength</u> will be less for lower coil factors.
<u>Time Between Tests</u>	[15..999 s]; resolution: 1 s The lower limit is dependent on <u>Magnetic Field Strength</u> ; its value will be higher at higher <u>Magnetic Field Strength</u> , reaching a maximum of 30 s at 800 A/m. If a number is entered which is less than the minimum time required to charge the circuit to the required <u>Surge Voltage</u> , the time will be replaced with the minimum time.
<u>Number of Tests</u>	[1..999] When the operator presses the START key, the system will execute the specified number of Charge and Surge cycles; the surge will occur automatically every <u>Interval Between Tests</u> , preceded by an audible warning.

## Preprogrammed IEC Standard Pulsed Magnetic Field Immunity Test Sequences

Each of the preprogrammed tests is a set of sequentially executed tests where most parameter values are predefined. Preprogrammed tests are based on the IEC Installation Class definitions.

There are two pre-stored IEC Standard test sequences, which test to different magnetic field strengths. The only adjustment the user can make is to the time between tests.

**Class 3 Test:** This test sets the magnetic field strength to 100 A/m and programs 5 pulses.

**Class 4 Test:** This test sets the magnetic field strength to 300 A/m and programs 5 pulses.

**Class 5 Test:** This test sets the magnetic field strength to 1000A/m and programs 5 pulses.

---

## PMF Waveform Verification

IEC 1000-4-9 requires that the simulator output be verified periodically, to ensure that the EUT is being tested at the proper test level. Waveform Verification takes place with the same setup as for EUT testing, but with the EUT removed.

Calibration requires a digital or storage oscilloscope with 100MHz bandwidth, a magnetic-field strength meter, and an inductive current probe and true-rms voltmeter capable of measuring 10 amperes peak with bandwidth exceeding 100Hz (the oscilloscope may be substituted for the voltmeter). KeyTek offers a magnetic-field strength meter, **CM-HMON**, for use in Verification. A Pearson<sup>7</sup> model 110 current transformer (or equivalent) may be used as the current probe.

The current probe is placed over one of the coil leads. The **EMCPro** is set for Power Frequency Magnetic Field testing, and programmed for a field strength of three A/m. The magnetic-field strength meter is placed in the center of the coil and oriented to achieve a maximum. This reading is recorded. The rms-reading of the current is recorded. The ratio of magnetic field to current is calculated and recorded.

The **EMCPro** is set for Pulsed Magnetic Field testing, and programmed for the proper field strength specified by the test level. A pulse is programmed and the peak current recorded via the oscilloscope. The ratio of magnetic-field to current -- calculated in the prior step -- is multiplied by the peak current -- measured in this step -- to obtain the actual magnetic field applied during test. This result is compared to the test level, and the coil factor adjusted accordingly: lower if the measured field strength is too low, higher if the measured field strength is too high. The measurement and adjustment may be repeated until the measured field strength is within acceptable tolerances of the desired field strength.

Alternatively, a peak reading magnetic field meter of bandwidth greater than 10MHz may be used. In this case the magnetic field may be measured directly (the current need not be measured).

---

The current waveform obtained in Pulsed Magnetic Field Testing is identical to that obtained in Surge testing. IEC 1000-4-9 refers to the wave as a 6.4/16uS wave; this is the result of a difference in definition of risetimes and duration. Per IEC 1000-4-9, the risetime is simply the time from 10% to 90% with no multiplier. The duration is simply the time from 50% of rise to 50% of fall.

---

---

<sup>7</sup> Pearson Electronics, Inc., 1860 Embarcadero Rd., Palo Alto, CA 94303 USA



---

# IEC 1000-4-11

## POWER QUALITY FAILURE Testing

### What is Power Quality Failure (PQF) Testing?

Dips and interrupts can occur on the AC power mains as a result of a fault in the distribution system such as an open circuit breaker or a sudden large load being turned on in the immediate vicinity. A power distribution system fault can cause a switch in the distribution grid to open and close a number of times, resulting in multiple interrupts to electrical and electronic equipment.

Electronic products are tested for immunity to dips and interrupts to insure their continued reliable operation if subjected to dips and/or interrupts on the AC power mains.

### General Guidelines for PQF Testing

The EUT is connected to the EUT outlet and powered. The EUT is allowed time to stabilize, and then a dip or interrupt is applied to the EUT. The duration and level of the dip is set by the test requirements.

The IEC 1000-4-11 sets three levels for PQF test; 70%, 40%, and 0% of mains voltage. KeyTek provides two types of zero-percent levels:

0%(OPEN) -- Represents a local (breaker or fuse) failure, with the AC mains at zero volts and in a high impedance state -- open.

0%(SHORT) -- Represents a remote (power system) failure, with the AC mains at zero volts and in a low impedance state -- short.

In addition to the standard test levels of 0%(open), 0%(short), 40%, and 70%, which are required for IEC testing and generated internally by the **EMCPro** an AUX input on the rear of the **EMCPro** allows testing to any level which the user-provides.

The **EMCPro** provides a PQF synchronization signal on the front panel; this connector will output a 5V pulse at the beginning of a PQF event (there is no pulse for Line Qualification tests).

---

## Testing Requirements per IEC 1000-4-11

Testing to IEC 1000-4-11 has the following requirements:

- Testing takes place in climatic conditions as follows:
  - Ambient temperature: 15 °C to 35 °C
  - Relative Humidity: 25 % to 75 %
  - Atmospheric Pressure: 86 kPa (860 mbar) to 106 kPa (1060 mbar)

Or other values of climatic conditions as given in the product specifications.

IEC 1000-4-11 requires the generator be capable of supplying peak inrush currents of up to 500A for 220V to 240V mains, and up to 250A for 100V to 120V mains. The **EMCPro** is designed to meet these levels, however -- due to building wiring capabilities -- the site where the **EMCPro** is being used may not meet the requirement.

The peak inrush current should be measured at the test site, using the circuit and method described in the **Waveform Verification** section.

If the **EMCPro** plus test site meets the inrush current requirement (500A peak for 220V to 240V mains, or 250A for 100V to 120V mains), it is not necessary to measure the EUT peak inrush current.

If the **EMCPro** plus test site does not meet the inrush current requirement, the test can still be performed as long as the EUT peak inrush current is less than the peak inrush current of the **EMCPro** plus test site. In this case, it is necessary to measure the EUT peak inrush current. The circuit and method for measuring EUT peak inrush current is described in the **Waveform Verification** section.

## User Defined PQF Test

The User Defined menu allows individual control of all test parameters required in PQF Testing; this allows testing at different levels, phase angles, number of tests, and time between tests.

A User-defined test is controlled by the parameters in the table below:

PQF Test Parameter	Range/Units
<u>Test Level</u>	[0% (open circuit), 0% (short circuit), 40%, 70%, External]  <u>Test Level</u> is the level of voltage during a test, as % of line voltage. The line voltage level before and after a test is the <u>Default/Standby Test Level</u> = 100%
<u>Starting Angle</u>	[0..360] ° of the line voltage waveform; resolution: 1°  <u>Starting Phase Angle</u> is the phase angle at which the dip or interruption begins
<u>Test Duration Units</u>	[cyc, sec], cyc is periods (cycles) of the Mains and sec is time in seconds
<u>Test Duration</u>	If <u>Test Duration Units</u> = "cyc": [0.1..3000.0] ; in the periods (cycles) of the line voltage waveform  If <u>Test Duration Units</u> = "sec": [0.01..60.00] s; where s is time in seconds  <u>Test Duration</u> is the duration of the dip or interruption, in either waveform periods or seconds
<u>Time Between Tests</u>	[10..999] s; resolution: 1 s
<u>Number of Tests</u>	[1..999]

## Preprogrammed IEC Standard PQF Test Sequences

Each is made up of a set of sequentially executed tests. The individual tests are similar to user defined PQF tests, except that all parameter values are predefined; none are changeable.

There are five Preprogrammed IEC Standard test sequences:

Test Sequence Name	Test Level	Test Duration
0% Open / 5 s	0% (open circuit)	5.00 s
0% Short / 5 s	0% (short circuit)	5.00 s
40% / 0.10 s	40%	0.10 s
70% / 0.01 s	70%	0.01 s
Combination	see right	<ul style="list-style-type: none"> <li>• Perform one IEC Standard "70%/0.01 s" test sequence</li> <li>• Perform one IEC Standard "40%/0.10 s" test sequence</li> <li>• Perform one IEC Standard "0% Short/5 s" test sequence</li> <li>• Perform one IEC Standard "0% Open/5 s" test sequence</li> </ul>

Each sequence has the following, common characteristics:

- Default/Standby Test Level = 100%
- Starting Phase Angle = 0° (and also 180° for Test Duration < 0.02 s)
- Interval Between Tests = 10 s
- Number of Tests = "N/A"

Each of the IEC Standard test sequences, except "Combination", is performed at the Test Level and using the Test Duration defined in the table above, as follows:

- 
- Start at the Default/Standby Test Level
  - Switch to the Test Level at Starting Phase Angle =  $0^\circ$ , and maintain for Test Duration
  - Switch to the Default/Standby Test Level, and maintain for Interval Between Tests
  - Switch to the Test Level at Starting Phase Angle =  $0^\circ$ , and maintain for Test Duration
  - Switch to the Default/Standby Test Level, and maintain for Interval Between Tests
  - Switch to the Test Level at Starting Phase Angle =  $0^\circ$  and maintain for Test Duration
  - Switch to the Default/Standby Test Level
  
  - If Test Duration is less than 0.02 s, then, in addition to the above:
    - Wait for Interval Between Tests
    - Switch to the Test Level at Starting Phase Angle =  $180^\circ$ , and maintain for Test Duration
    - Switch to the Default/Standby Test Level, and maintain for Interval Between Tests
    - Switch to the Test Level at Starting Phase Angle =  $180^\circ$ , and maintain for Test Duration
    - Switch to the Default/Standby Test Level, and maintain for Interval Between Tests
    - Switch to the Test Level at Starting Phase Angle =  $180^\circ$ , and maintain for Test Duration
    - Switch to the Default/Standby Test Level, and maintain for Interval Between Tests
  
  - Do not allow a new test sequence to start until Interval Between Tests has elapsed
  - End of test sequence

## **Other Preprogrammed Test Sequences -- Line Qualification**

See Waveform Verification Section

---

## PQF Waveform Verification

IEC 1000-4-11 requires that the simulator output be verified periodically. For Dip & Interrupt test simulators, it is necessary to verify the voltage transition levels, transition times to 100%, and the inrush current capability. Most modern oscilloscopes are capable of observing the voltage levels and transition times. Transition times are measured with a 100-ohm, 600-watt load. For verifying the inrush current, a bridge rectifier, suitably rated 1700uF capacitor, and appropriate current transformer (Pearson<sup>8</sup> model 110 or equivalent<sup>9</sup>) are required.

The Line Qualify test sequences meet the IEC 1000-4-11: 1994 standard for qualifying the “Test generator peak inrush current drive capability”. These test sequences require the use of a standard line qualification test load, “an uncharged capacitor whose value is 1700 μF in series with a suitable rectifier” (from IEC 1000-4-11: 1994, Clause 6.1.2). The two preprogrammed test sequences for verifying the peak inrush drive current capability of the test generator are:

Line Qualify 90°

Line Qualify 270°

Common characteristics of the “Line Qualify” test sequences are:

- Default/Standby Test Level = 0% (open circuit)
- Test Level = 100%
- Test Duration = 10 periods
- Interval Between Tests = 120 s (user selectable)
- Number of Tests = 1 (user selectable)

And the “Line Qualify” test sequence consists of the following steps:

Start at Default/Standby Test Level (open circuit)

Switch to Test Level at the Starting Phase Angle defined by the test sequence name

Maintain Test Level for Test Duration

Switch to Default/Standby Test Level (open circuit)

End test



### WARNING!


The Line Qualification Load will draw significant current; it should be plugged into the EUT outlet only when no voltage is present -- EUT switch OFF. DO NOT plug the Line Qualification Load into a live outlet as an arc may result which might damage the outlet.

The charged capacitor requires a time to discharge after each test. The time allowed should exceed 7 time constants (seven times value-resistor {in ohms} times value-capacitor {in farads}). Failure to allow sufficient time to discharge may give invalid readings. Allow the Line Qualification Load to discharge -- EUT switch OFF -- before handling.


---

<sup>8</sup> Pearson Electronics, Inc., 1860 Embarcadero Rd., Palo Alto, CA 94303 USA

<sup>9</sup> The Imon output of the EMCPro can be used for this measurement.

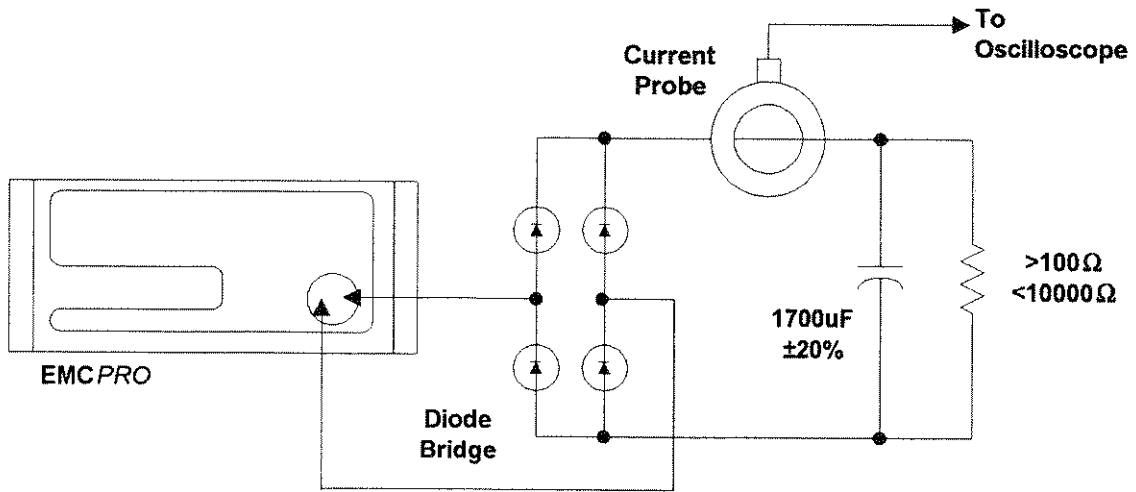

Line Qualification Test Setup -- Mains Peak Current

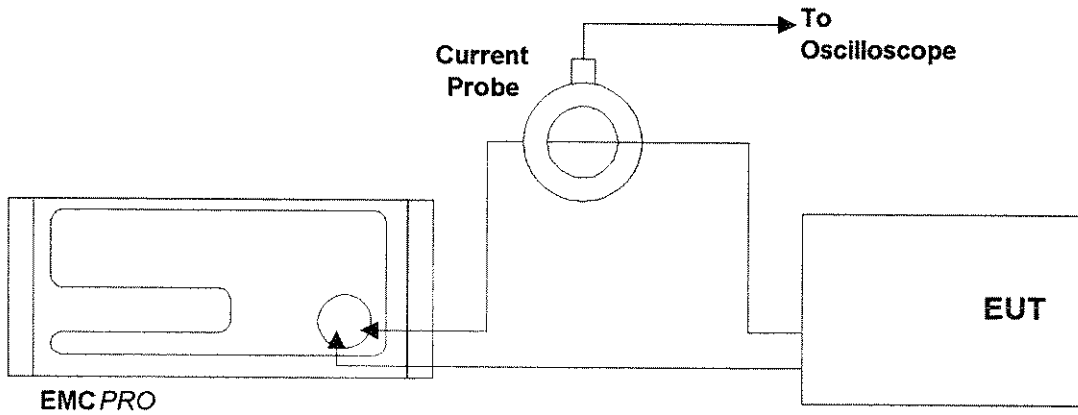

Line Qualification Test Setup -- EUT Peak Current

## Overview of the software

**CEWare** is the **EMCPro**'s PC control software. It provides full access to all the features and capabilities available from the **EMCPro** front panel, including running a single test and running a pre-defined test sequence.

Note: Version 2.0 (or greater) of **CEWare** is required for use with the **EMCPro**.

In addition, **CEWare** includes a number of useful features. It allows a user to:

- Create tests and easily edit them.
- Chain test sequences together. Multiple test sequences can then combine test types (e.g. do one or more Surge tests followed by one or more EFT tests, etc.).
- Store and recall tests and test sequences to disk.
- Log tests-- print or file a list of the tests which are executed.
- Develop tests off-line, and run in a simulation mode.

A Help file for the **EMCPro CEWare** is provided with the software which can be opened by clicking HelpContents on the menu bar. It provides complete operating instructions for the program; using the Help file while experimenting with the program is the recommended method for learning the software. Written instructions provided here are largely duplicated in the Help file.

The CM-SW option, available as a purchased **EMCPro** option, includes the **CEWare** program. It may be used on a Personal Computer (PC) running either Windows™ 3.1 or Windows95. The computer must have at least 16MB of RAM and a 80486/66MHz or faster processor. Screen transitions are slower on 486 processors, thus Pentium computers are recommended. **CEWare** is designed for an 800x600 display driver. You should select such a driver (or one with greater resolution) in your Windows configuration. On a driver with a smaller display, scrolling is necessary to see the entire application screen.

The CM-SW option includes an RS-232 to optical converter (the FC-11), a short RS-232 cable with a 9-pin D-shell connector, and a fiber optic cable with a duplex modular connector. The RS-232 connector connects to a Com port on your computer. The fiber optic cable connects to the **EMCPro** front panel; this connector is polarized and can only be inserted in one orientation: with the small tab on the connector facing right. Do not force the connector. The FiberCom option derives power from the RS-232 port of the computer -- no external power source is required.

---

# Basic Operations

The following steps will take you through major operating modes of the program and will acquaint you with the screens. Refer to the next section for full description of all the controls and displays on the screens. These steps can be run in simulation mode or with a **EMCPro** connected. If the **EMCPro** is connected and powered on, the application will send commands to the **EMCPro**.

## Starting the Program

- Start the **EMCPro** by powering it on and pressing a key to move beyond the warning screen.
- Start the **CEWare** program by double-clicking on the ICON in the **EMCPro** group on Windows 3.1, or running the program from the Start menu (PROGRAMS | **EMCPro** Software | **CEWare**) on Windows95.

## Defining a Test

- Click on one of the New Sequence buttons at the left of the Main Screen to create a new test.
- Select "User-defined" from the box on the New Sequence Definition screen. The other items on that screen are defaults (the same ones as on the **EMCPro** front panel) and can be left alone or changed, as you wish.
- Click "OK" on the Custom Sequence Wizard screen to accept the Wizard defaults. This screen allows you to create several tests of the same type quickly.
- Click "OK" on the Sequence Editor Screen to accept the test sequence. This screen allows you to manually edit the order of the tests or the test parameters.
- Back on the Main Screen, you now have one sequence defined and shown in the grid. You can return to the Sequence Editor at any time by double-clicking on the row or row number of the sequence you wish to edit.
- On the Menu bar at the top of the screen, select FILE | SAVE if you want to save your test.

## Running a Test

- Click on the RUN button to start the test. The grids on the Run Screen, and the Status Block at the lower right, will show the status of the executing tests.
- Hit the ABORT button to return to the Main Screen. After test completion, a notice is displayed, and return to the Main Screen is automatic on acknowledgment of the notice.
- Exit the application by choosing FILE | EXIT from the main application menu.



---

## Additional Operating Notes

- **Remote mode.** While the PC **CEWare** program controls the **EMCPro** the normal idle screen contains a "Comm: Remote; Status: Idle" indication if no test is running. When a test is active, a Run Screen (the same as from front panel control) will be shown on the front panel display. If the EXIT button on the front panel is pressed when in "Remote Idle," the **EMCPro** will no longer be controlled by the PC. This is not recommended. Termination of tests and remote control from the **CEWare** menu is preferable. (ESD test operation is a special case; see the next item.)

- **ESD operation.** The ESD test function is designed for maximum control at the ESD head. **EMCPro** operation puts the unit in a "Test Run" state, where it will stay until the user hits EXIT on the front panel. The same front-panel control is in place when running from **CEWare**. Leave the ESD run state by hitting EXIT on the front panel when all ESD pulsing is done. You may also select ABORT from **CEWare**, but this will terminate the entire sequence.

If your **EMCPro** does not have a front panel, the ABORT from **CEWare** is the only mechanism for stopping an ESD test. For this reason, putting an ESD test in a sequence with other test types is not recommended in that configuration.

During ESD tests, the user may perform more tests than are defined in the sequence definition; for this reason, the **CEWare** screen may show tests executed greater than the total tests, such as "140 of 100" pulses.

- **Mouse operations.** If running Windows 3.1 with the "snap-to" option enabled on the mouse driver (see the Mouse driver selections on the Windows Control Panel), the mouse cursor may jump when the mouse button is pressed. Turn off "snap-to," if it is enabled. Not all mouse drivers support "snap-to."

- **Editing pre-programmed surge tests.** Some of the pre-programmed surge tests (pre-qualification and Level 1) include voltages which are below the normal limit for surge user-defined tests. These tests will run as pre-programmed tests, but not as user-defined tests. If you edit these pre-programmed tests and attempt to run without changing the voltages, **CEWare** will report errors at each voltage below the normal limit. If these low-voltage, pre-programmed tests are edited, be certain to remove or change all the voltages below the 200V limit.

- **Test timing counts.** The test count displayed on the **CEWare** screen is a combination of values from **CEWare** timing and firmware timing. It may sometimes change quickly, faster than a normal clock, or lag the front panel count, due to communication delays. The test is being executed by the firmware, and the front panel has the most current information for each test. Only **CEWare** supports user-defined sequences and combinations of sequences; timing information is summarized in the Sequence List Status block, as described in other sections of the manual.

---

## CEMaster/EMCPro Differences

### CEWare Support of EMCPro and CEMaster differences

The standard test sequences supported on **CEMaster** and **EMCPro** are not identical. This is largely due to the higher voltages and additional test types of the **EMCPro**. While CEWare version 2.0 supports both products, there are certain incompatibilities when using these standard sequences.

### Using CEMaster standard sequences with the EMCPro

Most standard sequences created in CEWare for use on the **CEMaster** can also be used on the **EMCPro**. The exceptions are those containing at least one of the following Surge (1.2/50) sequences:

- PreQual A*
- PreQual B*
- Class 1 Fast*
- Class 1 Full (formerly called Class 1 Complete)*
- Class 2 Full (formerly called Class 2 Complete)*

While neither of the **CEMaster** prequalification sequences are available on the **EMCPro**, the *Class 1 Fast* sequence is the same as the **EMCPro** sequence *Class 1 Full*, and therefore a direct substitution can be made. Note, however, that the new suite will not run on a **CEMaster**. Also note that the **CEMaster** *Class 1 Full* and *Class 2 Full* sequences are not the same as those sequences with the same names on the **EMCPro**.

### Using EMCPro standard sequences with the CEMaster

Many standard sequences created in CEWare for use on the **EMCPro** can also be used on the **CEMaster**. The exceptions are those containing at least one of the following sequences:

- EFT Class 4*
- HPulse Class 5*
- Surge (1.2/50) Class 1 Full*
- Surge (1.2/50) Class 2 Full*
- Surge (1.2/50) Class 4 Fast*
- Surge (1.2/50) Class 4 Full*
- Surge (10/700), all sequences
- Surge (Ring), all sequences

Note that the **EMCPro** *Class 1 Full* and *Class 2 Full* sequences are not the same as those sequences with the same names on the **CEMaster**. However the **EMCPro** *Surge(1.2/50) Class 1 Full* sequence is the same as the **CEMaster** sequence *Surge (1.2/50) Class 1 Fast*, and therefore a direct substitution can be made. Note, though, that the new suite will not run on an **EMCPro**.

---

## Changing Program Settings

Program settings - defaults - affecting communications, data logging, and user-defined messages, may be changed from the menu bar; the setup option. See the Menu, Toolbar, and Status Bar section for more detail.

• **Viewing, editing, and printing test reports outside CEWare.** Test logs may also be viewed, edited, and printed using a word processor. The following document format controls are appropriate for MicroSoft Word. Equivalent margin and font selections are likely to be necessary from other word processors.

1. Start MS Word and select the text log file you wish to print from FILE

- OPEN.

2. Select all of the text in the document

3. Select FORMAT - FONT

- Select Font = Courier New, MS LineDraw, or Lucida Console
- Select Font Style = Regular
- Select Size = 10
- Select OK

4. Select FILE - PAGE SETUP

- Set Margins Left = 0.9"
- Right = 0.9"
- Top = 1.0"
- Bottom = 1.0"
- Select OK

5. If you wish to Print, select FILE - PRINT

# CEWare in Detail

## Screens and Organization

CEWare uses five screens to create, edit, and run tests. The material on the screens is described in the following sections. This information is also contained in the Help file.

**Main Screen** -- The overview screen; used to create and run tests.

**New Sequence Definition Screen** -- Used to define a test sequence, selecting pre-programmed or custom (user-defined) tests.

**New Custom Sequence Wizard Screen** -- If a User Defined test sequence is selected, the Custom Sequence Wizard will help define the sequence of tests.

**Sequence Editor Screen** -- Used to modify a test sequence.

**Run Screen** -- Shows Test Status information while tests are running.

The screenshot displays the 'Run Screen' interface. At the top, there is a toolbar with icons for navigation and control. Below the toolbar, the main window is titled 'Sequence List Description'. On the left side, there is a 'New Sequence' panel with several test sequence icons: ESD, EFT, Surge 1.2/50, HPower, HPulse, PQF, and Surge Ring. The central area contains a 'Sequence List' table with the following data:

Sequence	Type	Sequence Description
1	PQF	Standard
2	Srg 1.2/50	Standard
3	EFT	Standard

Below the table, there are two status panels: 'Sequence List Status' and 'Present Sequence Status'. The 'Sequence List Status' panel shows: Sequence 0 of 3, Duration 0, Elapsed Time 0, Repeat Count 1 of 0. The 'Present Sequence Status' panel shows: Test 0 of 0, Duration 0, Elapsed Time 0, Repeat Count 1 of 1. At the bottom of the screen, there are several status indicators: Communication: DISCONNECTED LOCAL, Run State: IDLE, and Logging: OFF. There are also control buttons for 'Run', 'Abort', 'EUT POWER OFF', 'Break', and 'Comment', along with checkboxes for 'Auto Pause' and 'Repeats'.

---

## Main Screen

The Main Screen is the screen used to create tests, load or save tests, and run tests.

To create a new test, click on one of the seven test buttons, left-center on the screen. To load an existing test, click on the Toolbar or Menubar at the top of the screen. To Run a test click on the RUN button at the bottom left of the screen. The following sections describe the information and the controls on the Main Screen.

### Toolbar

The toolbar at the top of the screen supports some system-level operations. It is described in detail in the section on Menu, Toolbar, and Status Bar, which appear on several screens.

### Test Status Block

When on the Run Screen, the Test Status Block shows which test is currently executing, and shows duration and elapsed times. While displayed on the Main Screen, this block is updated when a test sequence is selected or deselected on the Sequence List grid. It is described in detail in the section on the Run Screen.

### Test Control Block

The test control block has control buttons to start, stop, and control tests.

- RUN                    The Run button starts the Test. Once the test is running, the Run button becomes the Pause button.
- PAUSE                (Only enabled on Run Screen) -- Click the Pause button to temporarily halt the test.
- RESUME              (Only on Run Screen, when in Paused state) -- Click to resume a paused test.
- ABORT                The Abort button Halts the test.
- BREAK                The Break button 'breaks' out of loops.  
  
When you click the Break button, if the Present Sequence Status has a repeat count greater than one, it drops to one. Any test presently executing continues to completion, but at completion the present test ends.  
  
If the Sequence List Status has a repeat count greater than one, it drops to one. Any test presently executing continues to completion, but at completion the present test ends; at completion of all tests in the present sequence, the present sequence ends.
- COMMENT            The comment button is only active when logging is set to ON. This Comment button allows definition of a user comment while tests are running. The comment can then be inserted into the log file at any instance the user chooses by selecting the OK button on the comment entry window.

---

- **AUTO PAUSE/REPEATS Checkboxes**

Enable steps and defined sequence repeats.

When checked, AUTO PAUSE will enable any pauses defined in the Sequence Editor. At each pause the operator must click the OK button on a Windows prompt box to continue the test. When un-checked, any pauses defined in the Sequence Editor are ignored. When checked, REPEATS will allow any repeats defined in the Sequence Editor and in the main menu. When un-checked, any repeats are ignored; each test and sequence will execute exactly one time. (This is the mechanism for single-stepping, used in coordination with the Pause column on the Sequence Editing screen.)

- **EUT POWER STATUS**

The EUT Power status button shows the EUT status. The EUT power may be turned off from the computer by clicking this button. When off, the EUT Power can only be turned on from the **EMCPro**, by turning the EUT switch ON, or toggling OFF and ON.

### Sequence List Grid

The Sequence List Grid shows which test sequences have been defined (or loaded with the current file). The grid allows editing the sequence during the definition and editing phases. A yellow highlighted bar identifies the test to be edited when using CUT, COPY, and PASTE.

- **To Edit a Test Sequence:**  
Double-click on the gray, numbered, row-header cell to the left of the test you want to edit, or anywhere in the row of that test. The Sequence editor will open.
- **To Add a Test Sequence to the end of the sequence list:**  
Deselect any selected Test Sequences by clicking the button in the upper-left corner of the grid. Then, click a test type button.
- **To Insert a Test Sequence:**  
Click the gray numbered cell to the left of the test you want to insert the new sequence in front of. Then select a test type by clicking a test type button.
- **To Delete a Test Sequence:**  
Click the gray numbered cell to the left of the test you want to delete. Then click the Cut button from the toolbar.
- **To Move a Test Sequence:**  
Click the gray numbered cell to the left of the test you want to move. Click the Cut button from the toolbar to remove this test. Click the gray numbered cell to the left of the test you want to insert the cut sequence in front of. Then click the paste button from the toolbar to insert the test.

---

### Test Type Controls

These 7 buttons at the left of the Main Screen select a test type to create. There are 8 different immunity tests available, in accordance with European Norm requirements and the controlling, basic EMC immunity standards of:

IEC 1000-4-2	ESD
IEC 1000-4-4	EFT
IEC 1000-4-5	Combination and Telecom Wave Surge
IEC 1000-4-8	Power Frequency Magnetic Field
IEC 1000-4-9	Pulse Magnetic Field
IEC 1000-4-11	Dip and Interrupt
IEC 1000-4-12	100kHz RingWave for AC Mains

The tests available on your system will depend on the options installed in your **EMCPro**. If a test is not available, the corresponding test button will be grayed out, and cannot be selected. The legend on the last button will depend on the surge option installed in the system.

### Repeat Control

The repeat control sets how many times the sequence shown in the Sequence List grid will be executed. Click this control and enter a number.

### Test Description

If a test is loaded from a file, the description box will contain the text description filed with the test. If a new test is created, enter a description of the test in the description box for inclusion in reports and logfiles, and to be saved with the test.

### Tool Bar

The toolbar holds icons for common tasks, allowing you to select that task with a single mouse-click. See the section below on the Menu, Toolbar, and Status Bar.

- File Icons -- The file icons create a new test sequence, load an existing test sequence, or save the current test sequence. If you attempt to create a new sequence or load an existing sequence, you will be prompted to save any existing work.
- Edit Icons -- The CUT, COPY, and PASTE icons allow you to edit the test sequence grid. These icons are also found in the Sequence Editor.
- The Printer icon will print the test sequence.

### Starting a Run

When you wish to execute the presently defined sequence list, select the Run button in the Test Control area. A Windows message box will appear to inform you if you are doing a Local/Simulation run. If you are about to do a Remote run (connected to a **EMCPro**) no warning is given.

If Logging is enabled, a Run-Time Logging Information screen will appear. In it you will see the header information that will appear in the log report(s). This information can be edited.

You may edit the 60 character log report header line or the 40 character operator name. There is a 60 character field for a description of the equipment under test and a text entry field where you can make any comments regarding the run before you begin. The comment will appear after the header on the first page of the log text report.

Enter up to 8 characters for the file name for either or both of the log report types selected. This must be a valid 8 character DOS filename. The file paths and extensions are shown for reference only and are not editable in this window.

**Run-Time Logging Information** [X]

LOCAL/SIMULATION RUN: SW v1.10 Sim v1.10 Seq v1.01 Rul v1.01 Str v1.01

Company / Report Header Line: KeyTek CEWare/CEMASTER Compliance Tester Log Report

Operator: Fredrick W. Flintstone

Equipment Under Test:

Comment:

**Text Reports**

Path	File Name	Extension
C:\CEMASTER\LOGFILES	RUFUS	.TXT


**Export Reports**

Path	File Name	Extension
C:\CEMASTER\LOGFILES	CEMASTER	.EXP

Buttons: OK, Cancel

**Run-Time Logging Information Screen**



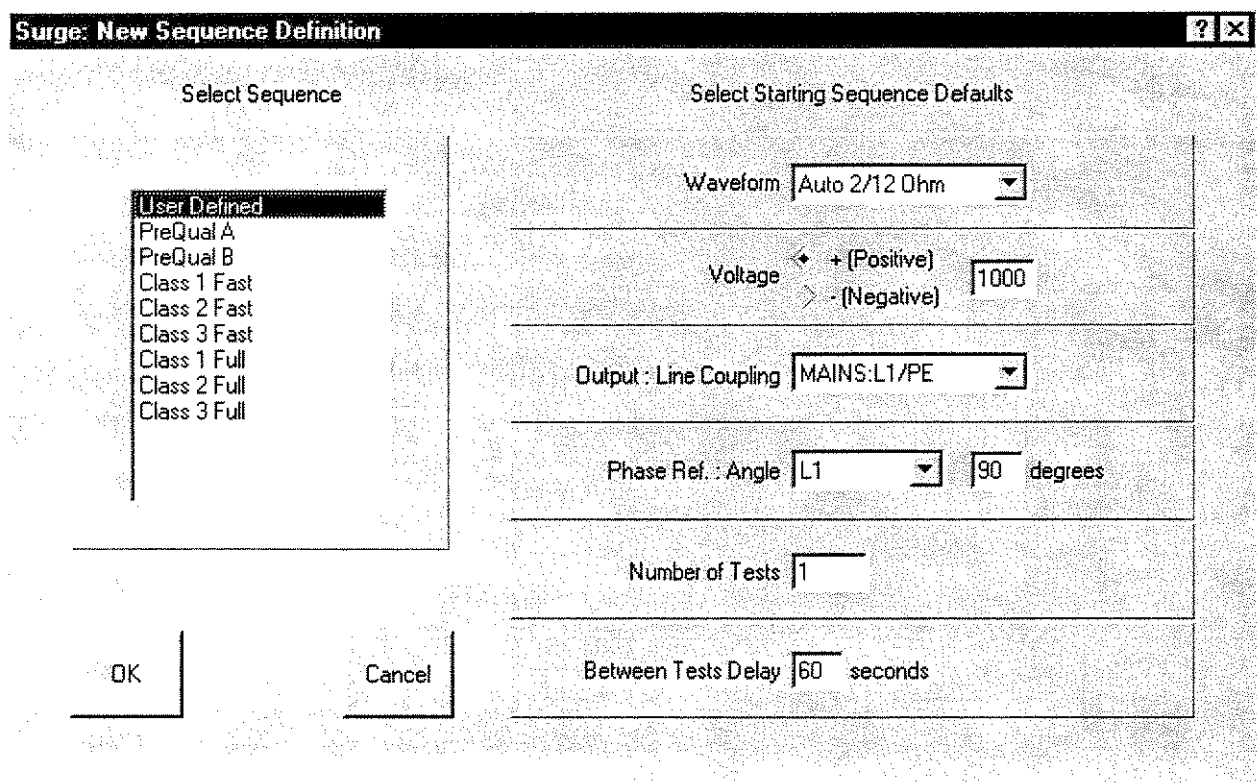


### New Sequence Definition Screen

#### New Sequence Definition Screen

The New Sequence Definition Screen is opened when you create a new test (by clicking on one of the test type buttons from the Main screen).

The list box to the left of the screen shows available sequences. The User Defined sequence gives you the most control over the test, allowing you to define all of the Sequence Defaults shown on the right side of the screen. The other options shown -- which vary by test type -- are test sequences which the **EMCPro** has stored and available. These sequences speed set-up and execution of commonly performed IEC test sequences by setting and locking many of the defaults. Locked defaults will be grayed, and cannot be selected. The standard test sequences for each test type are described in the **EMCPro** manual.

To continue, click one of the sequences shown. If the Sequence Defaults to the right of the screen are enabled, you can select one or more of the Defaults. Finally, click OK.

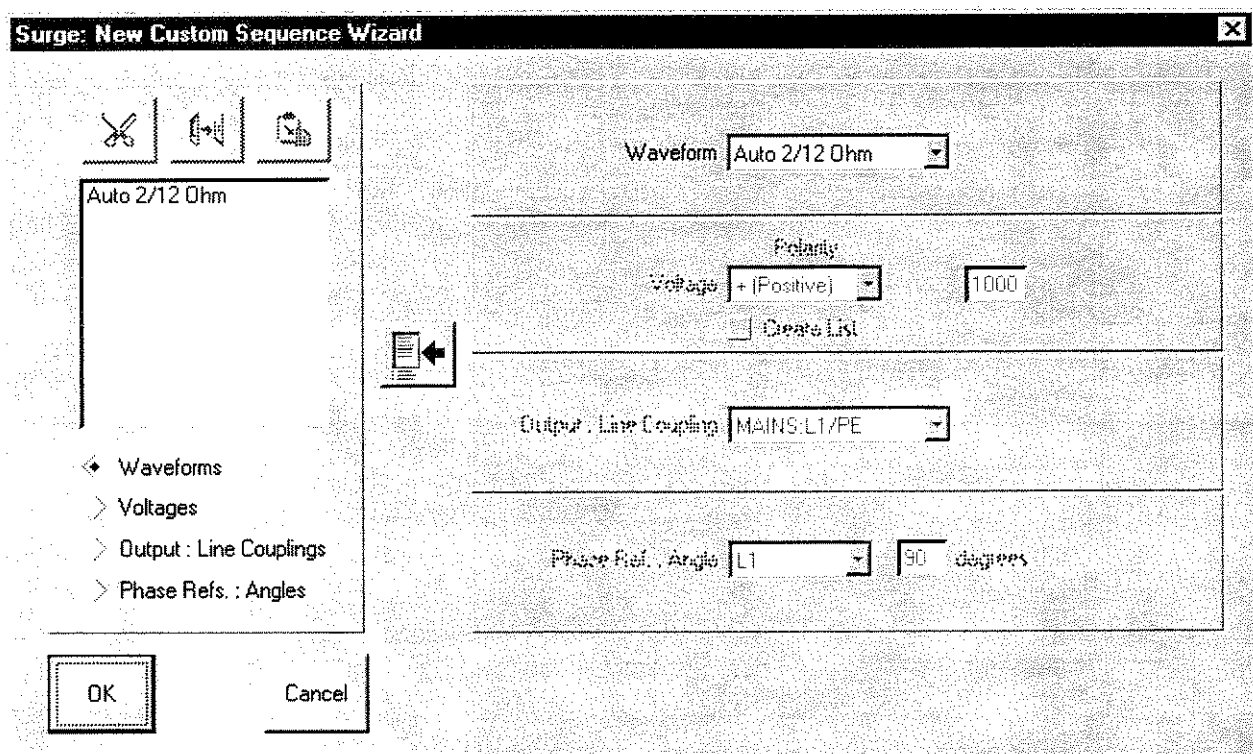

**New Custom Sequence Wizard Screen**

## New Custom Sequence Wizard Screen

The New Custom Sequence Wizard screen quickly creates test sequences. The Wizard is run automatically whenever you select a User Defined Sequence in the New Sequence Definition Screen. The Wizard allows you to create lists of one or more parameters, then forms all combinations of these parameters to quickly create a large number of tests. When you click OK, the Wizard closes and the Sequence Editor opens for fine editing of test parameters.

To use the Wizard, select one of the radio button options at the bottom left of the screen, or click within any parameter definition box to the right of the screen. The defaults in the combo boxes are those you selected from the New Sequence Definition Screen. Make a parameter selection, then click the Insert button (to the left of the parameter definition boxes) to copy the selection into the list box. You can change list boxes using the radio buttons below the list box, and edit the list box using the CUT, COPY, and PASTE buttons above the list box.


For example, if you click Voltages, and insert 250V, 500V, and 1000V, then click Output and select L1-L2 and L1-PE, when you exit the Wizard, the Wizard will create six tests:

- L1-L2 at 250V
- L1-L2 at 500V
- L1-L2 at 1000V
- L1-PE at 250V
- L1-PE at 500V
- L1-PE at 1000V

If you want to create a User-Defined test sequence with a single test, simply click the OK button to exit the Wizard and open the Sequence Editor.

### Sequence Editor Screen

The Sequence Editor is opened after selecting a test sequence from the New Sequence Definition Screen, or by double-clicking an existing test from the test on the Main Screen. The sequence editor gives you fine control over what tests are performed and all options. If you wish to execute a predefined test with no changes, you should simply click on the OK button. If you make any changes in a predefined test, the test will be re-defined as a User Defined test.

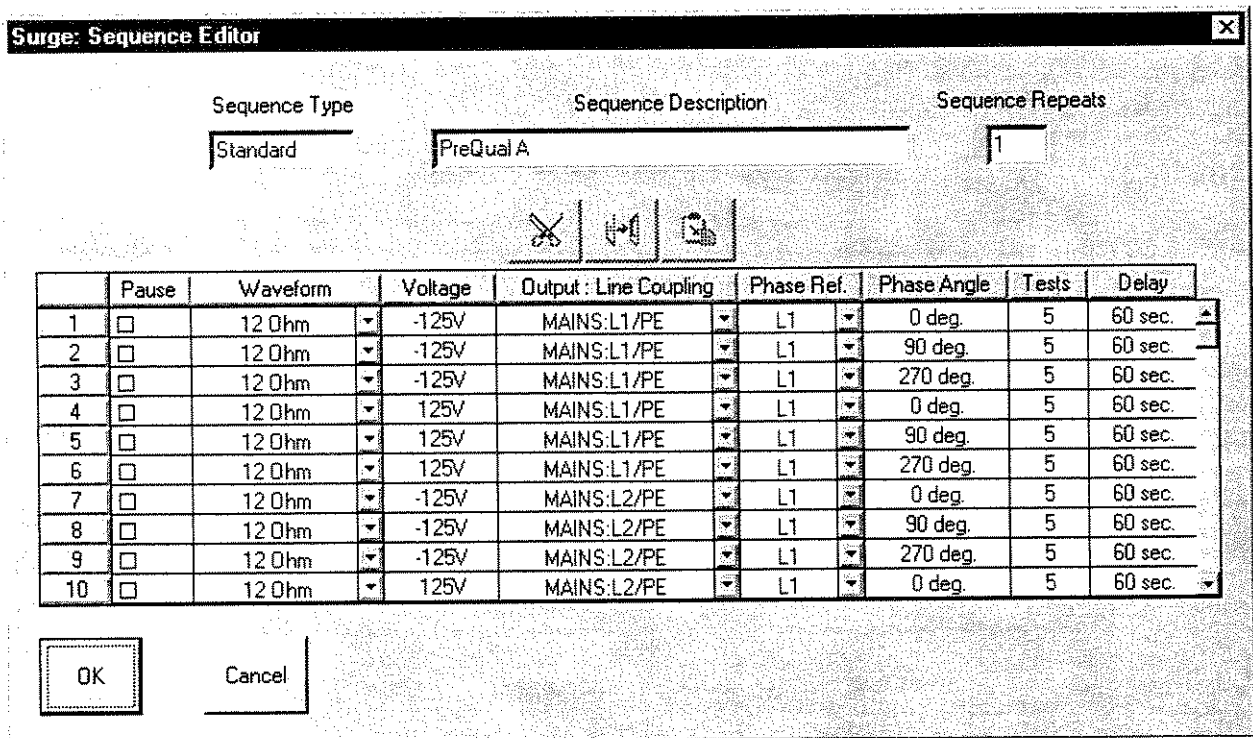

Sequence Editor Screen

---

## Sequence Description Grid

The Sequence Description Grid shows which tests have been defined in a sequence. It supports the editing process on the Sequence Editing Screen as well as allowing the data to be changed in any individual cell. Basic test editing is allowed on any test in the grid. Text cells can be changed by selecting a cell, deleting the current entry, and typing a new one. Cells that support a list of legal values have a standard Windows drop-down list controlled by the drop-down button at the right of the cell. Open the list and select a new value to change it. Additional editing controls that affect more than one cell are also supported and are described in more detail below.

- **PAUSE or PAUSE AND DISPLAY MESSAGE Control**

The PAUSE column of this grid allows single-stepping or automatic stopping at any test in the sequence. Check the box in the row of the test where you wish to pause. (The pause will occur before the test executes.) Make sure that the Auto Pause box is checked, on the Main Screen, before the test starts. The PAUSE box for all tests in a sequence may be set with the technique described in this section for changing an entire column.

To set or reset the PAUSE box, use a single left button click of the mouse to select the PAUSE cell then use single left button clicks to set or reset the check-box in the cell. A message can be displayed during a PAUSE - see the Message Selection section.

A yellow highlighted bar identifies the test to be edited when using CUT, COPY, and PASTE, which act on entire test rows.

- **To Delete a Test Sequence**

Click the gray, numbered cell to the left of the test you want to delete. The entire row will be highlighted. Then click the CUT button from the toolbar.

- **To Move a Test Sequence**

Click the gray, numbered cell to the left of the test you want to move. Click the CUT button above the grid to remove this test. Click the gray numbered cell to the left of the test that will follow the moved test. Then click the PASTE button from the toolbar to insert the test.

- **To Copy a Test Step**

Click the gray, numbered box to the left of the test you want to copy; the entire row will be highlighted. Click the COPY button.

- 
- To Paste a Test Step

After a Cut or Copy operation, click the gray, numbered box to the left of the test you want to insert in front of; the entire row will be highlighted. Click the PASTE button. NOTE: To select a block of rows, hold the [Shift] key when left-clicking; to select multiple single rows, hold [Cntrl] key when left-clicking.

The Sequence Editor allows several special editing operations in addition to the normal Cut and Paste Operations. These operations take place over all or part of a column. This allows you to change many tests with a single editing step.

- To change an entire column

Click one cell within the column you want to change. Then, click the gray column header at the top of the grid. All cells in the column will be highlighted.

Press ENTER. The cell you highlighted will open for editing. Select a new value and press ENTER (if this is a numeric cell, type in a new value and press ENTER; if this is a check box, press ENTER to toggle).

All cells in the column -- and thus all tests within this sequence -- will take on the new value you entered.

- To change all entries in a range within a column

Click the first cell in the range within the column you want to change. Then, hold down the shift key and click the last cell in the range you want to change. All cells between the first and last cells will be highlighted.

Press ENTER. The last cell you highlighted will open for editing. Select a new value and press ENTER (if this is a numeric cell, type in a new value and press ENTER; if this is a check box, press ENTER to toggle).

All cells in the range will take on the new value you entered.

When you change a column, other columns may change as a result. These changes will always be 'legal' -- that is, the test will run with the resulting change, and you will not get an error. But the changes may not be uniform. Check the other columns to be sure the tests will run the way you want them to.


### Keyboard Editing

The grid can be edited using the keyboard cursor keys, Tab, and ENTER. Press Tab until the grid is selected -- the highlighted cell within the grid will have a dotted selection-box drawn inside it. Use the cursor keys to select a cell to edit. Press ENTER to open the cell. If the cell is

a drop-down box, use the cursors to select an option. If the cell is numeric, type in a new value. Press ENTER to accept the change.

### Message Selection Grid


To assign a message to be displayed during a run-time pause, double-click the left mouse button on the desired PAUSE cell. This will bring up the Message Selection window where a single 80-character message may be selected from 200 available messages. See message editor section on adding or modifying messages.

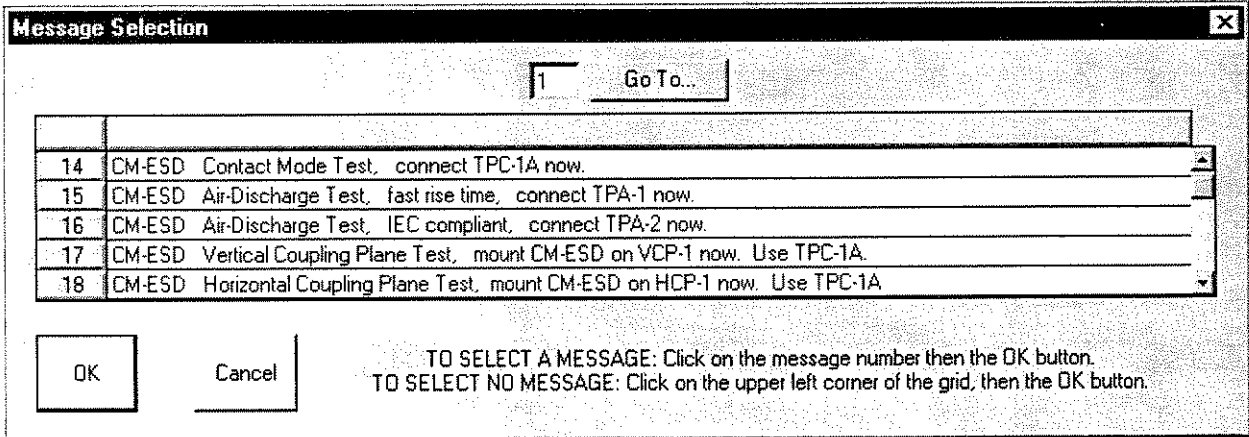

### Message Selection Screen


Use the right scroll bar to scroll through the 200 messages or enter a specific message number in the Go To... edit box then click the Go To... button.

Select the desired message by clicking on the message number button to the right of the message, then click OK.

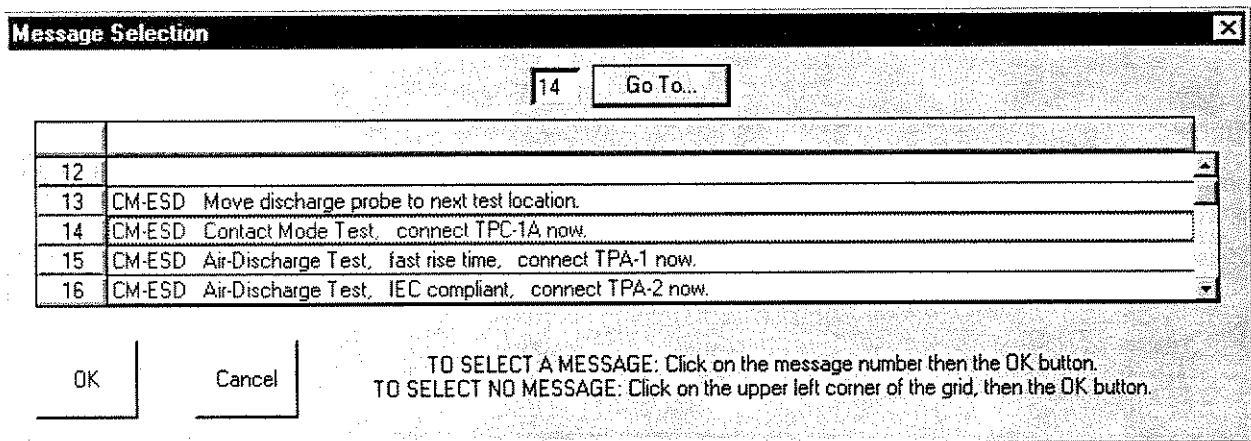

### Message Selection Screen, with message selected

When OK is selected, the Message Selection Window closes, and the message number is pasted in the PAUSE cell of the Sequence Editor Grid.

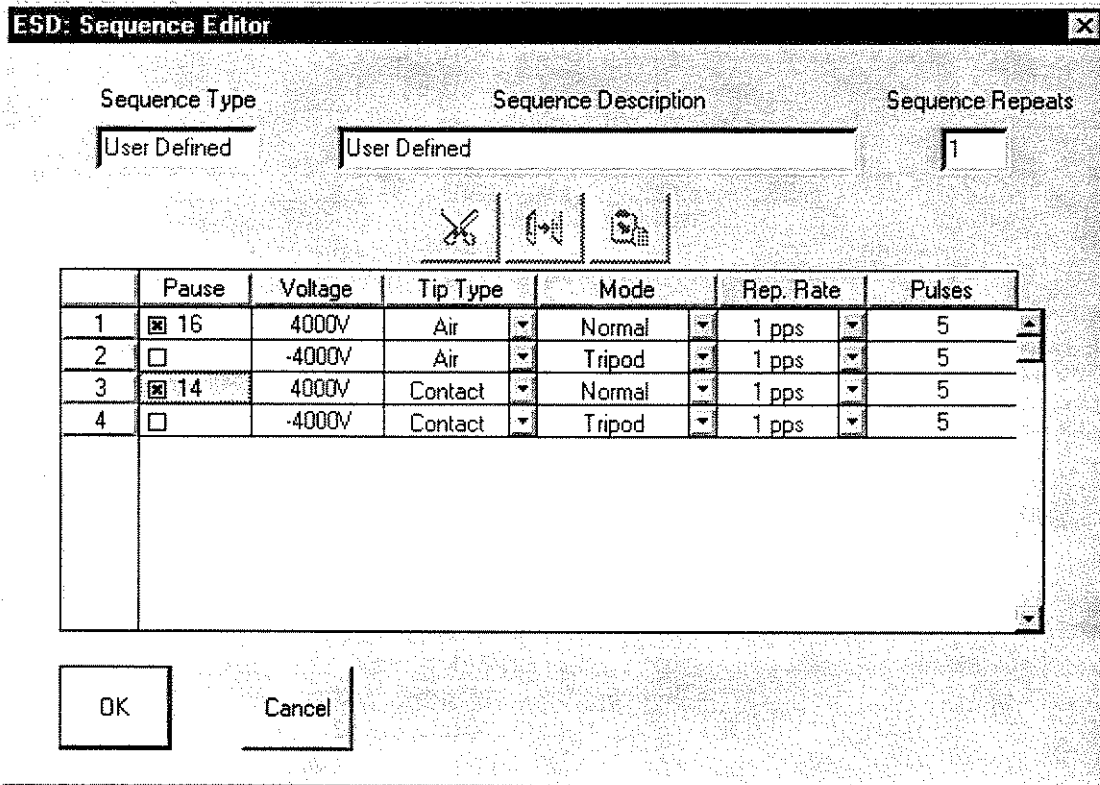

**ESD: Sequence Editor Screen**

To remove a message from being displayed during pause, double-click the left mouse button on the desired PAUSE cell. This will bring up the Message Selection window where the selected message will be displayed highlighted.

Deselect the message by clicking on the upper left corner button on the Message Selection grid, then click OK.

NOTE: The Message Selection grid does allow editing of message text but does not allow Cut, Copy and Paste operations.

## The Run Screen

The Run Screen interface displays the following components:

**Sequence List Description**

Sequence	Type	Sequence Description
1	Srg 1,2/50	Standard
2	EFT	Standard

**Present Sequence**

	Pause	Waveform	Voltage	Output : Line Coupling	Phase Ref.	Phase Angle	Tests	Delay
1	<input type="checkbox"/>	12 Ohm	-125V	MAINS:L1/PE	L1	0 deg.	5	60 sec.
2	<input type="checkbox"/>	12 Ohm	-125V	MAINS:L1/PE	L1	90 deg.	5	60 sec.
3	<input type="checkbox"/>	12 Ohm	-125V	MAINS:L1/PE	L1	270 deg.	5	60 sec.
4	<input type="checkbox"/>	12 Ohm	125V	MAINS:L1/PE	L1	0 deg.	5	60 sec.
5	<input type="checkbox"/>	12 Ohm	125V	MAINS:L1/PE	L1	90 deg.	5	60 sec.

**Control Buttons:** Pause, Abort, EUT POWER OFF, Break, Comment.

**Sequence List Status:** Sequence 1 of 2, Duration 1:00:00, Elapsed Time 0:00:00, Repeat Count 1 of 1.

**Present Sequence Status:** Test 5 of 5, Duration 0:00:00, Elapsed Time 0:00:00, Repeat Count 1 of 1.

## The Run Screen

The Run Screen is displayed while tests are executing. A Present Sequence grid control is added to the screen, along with the Sequence List grid control. Together they describe the current set of tests being run.

### Sequence List Grid

This list of sequences is the same as shown on the Main Screen, and shows the presently defined set of test sequences. A yellow highlighted bar indicates the test sequence that is presently executing.



---

## Present Sequence Grid

The Present Sequence Grid is displayed when running tests. The grid shows all the parameters of the present test sequence, which consists of one or more tests. It is essentially the same information presented on the Sequence Edit screen. A horizontal highlighted bar across the grid identifies which test of the sequence is running.

## Test Status Block

The Test Status Block at the lower right of the Run Screen shows which test is currently executing, test duration, and elapsed times. It contains two display areas: one for the Sequence List, and one for Present Sequence -- the one that is currently executing. The two sets of data are similar. The Sequence List Status summarizes statistics for the entire set of sequences, and the current sequence within that list. The Present Sequence summarizes information about the current test within the present sequence.

- Sequence List Status

Sequence	The sequence that is running, out of the total number of sequences.
Duration	The duration shown is the estimated time required to complete the entire sequence, excluding time for pauses. The time format is hours:minutes:seconds.
Elapsed Time	The elapsed time is the total time from the start of the test to the present time.
Repeat Count	These fields show the present loop count, and the total list count for the sequence. The total reflects the value from the List Repeats field on the Main Screen.

- Present Sequence Status

Test	These fields identify which test is running out of the total number of tests in the present sequence.
Duration	The duration shown is the estimated time required to complete the Present Test Sequence. The time format is hours:minutes:seconds.
Elapsed Time	The elapsed time is the total time from the start of the present sequence to the present time.
Repeat Count	These fields show the present loop count, and the total list count for the sequence. The total reflects the value from the Sequence Editor, Sequence Repeats field.

## Test Control Block

This set of buttons is the same as on the Main Screen and is described in that section. Buttons may be enabled or not, depending on the state of the system and the software.

---

## Menu, Toolbar, and Status Bar

These areas appear on both the Main and Run Screens.

### Menubar

The menubar performs actions, sets options and preferences, and accesses the help file. The menu options are described below.



File Edit Setup Enable System Help

### Menubar Selections

#### File Menu

The File menu supports loading and saving of test files, and exit from the application. The default extension used for test sequence files is .SEQ.

- File | New

Delete any present tests and prepare for creating a new test. If you have tests defined and have not saved them you will be prompted to save the tests before continuing.

- File | Open

Load an existing test file. The File Common-Dialog box will open, allowing you to click on a file to load. If you have tests defined and have not saved them you will be prompted to save the tests before continuing.

- File | Save, Save As

The Save command will save the present test to a disk file. If the test was loaded from disk, the test will be written to the same file. If the test is a new test, you will be prompted for a path and filename to use in saving the test.

The Save As command will prompt you for a path and filename to use in saving the test. Use this command to create file copies of tests, or new tests based on the old ones that you have edited.

- File | Print Sequence, Print Log, Print Setup

The Print Sequence command will print the present Sequence List.

The Print Setup command controls the printer, selecting which printer is used, which font is used, and paper orientation. Print Log will allow the user to select and print a Log file.

- File | File Select

This section holds the last four files you opened / saved. You can quickly load a prior file by clicking one of these selections or typing the corresponding number

- File | Exit


This selection exits from the application.

### Edit

The Edit menu allows keyboard selection of the CUT, COPY, and PASTE selections that are also accessible from the Toolbar. In addition, there is a DELETE selection which does a destructive cut of selected data.

### Setup

The Setup menu is where the user may select and set parameters for run time operation or report generation. The items on the setup menu are:

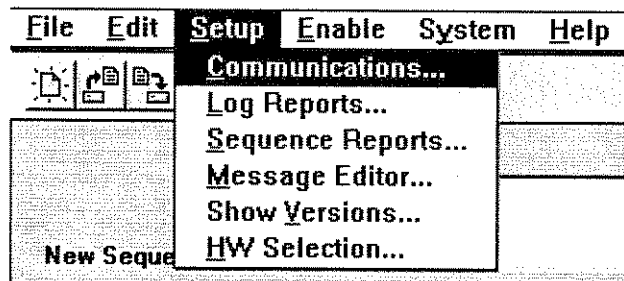

Setup menu

- Communications

The user may select the COM port to set up communications with an **EMCPro**. **CEWare** allows selections (COM1 - COM4) and automatically detects which ports are available on the system. The default selection is COM1. Other communication parameters, although shown, are fixed.

Setup: Communication Parameters	
Serial (COM) Port	
<input checked="" type="radio"/> COM1	<input type="radio"/> COM3
<input type="radio"/> COM2	<input type="radio"/> COM4
Baud Rate (bps)	Parity
<input checked="" type="radio"/> 9600	<input type="radio"/> Odd
<input type="radio"/> 19200	<input type="radio"/> Even
<input type="radio"/> 38400	<input checked="" type="radio"/> None
Data Bits	Stop Bits
<input type="radio"/> 7	<input checked="" type="radio"/> 1
<input checked="" type="radio"/> 8	<input type="radio"/> 2

**Communication Parameters Screen**

- Log Reports

Log Reports allows the user to select the type of logging reports to produce: Text Reports or Export Reports. For each type of report, you may define your own file extension and path or you may accept the defaults (you will be asked to enter a log report file name at run time). The file extension must be a (up to) 3 character valid DOS file extension. The path must be a valid DOS path of up to 60 characters in length.

You may also define your own header line that will appear as the first line in the header of all Log reports. A default report header is supplied. You may enter a new report header of up to 60 characters.

A 40 character field is supplied where you may enter an operator name that will also appear on the Log reports.

**Setup: Log Reports**

**Text Reports**

Extension:  Path:

**Export Reports**

Extension:  Path:

**Company / Report Header Line**

**Operator**


OK  
Cancel  
Defaults

**Log Reports Screen**

- Sequence Reports

---

Sequence Reports allows the user to define his own header line that will appear as the first one in the header of all Sequence List reports. All other data for the Sequence List report is fixed. A default report header is supplied. You may enter a new report header of up to 60 characters.

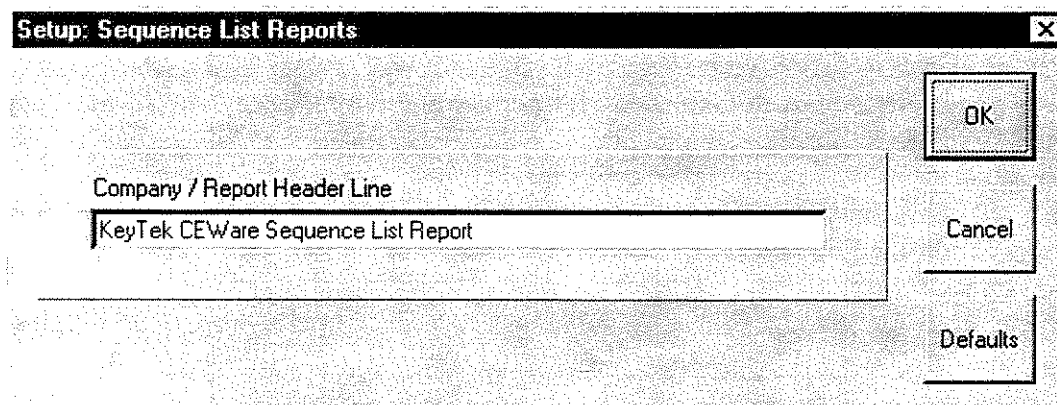

**Sequence List Reports Screen**

- Message Editor


The Message Editor allows you to define up to 200 messages that may later be attached to Auto-Pause controls on the test edit screens for display to an operator at run time. Use

the scroll bar control on the right side of the message grid to scroll through the 200 messages. Each message may be up to 80 characters (maximum) in length. A set of default messages is supplied for use with several optional components available for use with the **EMCPro**. These default messages may be redefined if you desire.

To define a message, click within a message cell to highlight it (*green* highlight), then click a second time to enter "edit mode" for the cell. Enter the desired message text then press **Enter**.

To select messages for CUT, COPY, and PASTE operations, click the message number cells on the left side of the message grid. This will highlight the message in *yellow*. Multiple messages may be selected by holding the **Ctrl** key while clicking, or a block of messages may be selected by holding the **Shift** key while clicking after the first message in the block has been selected.


To deselect all messages, click the button in the upper left corner of the message grid.

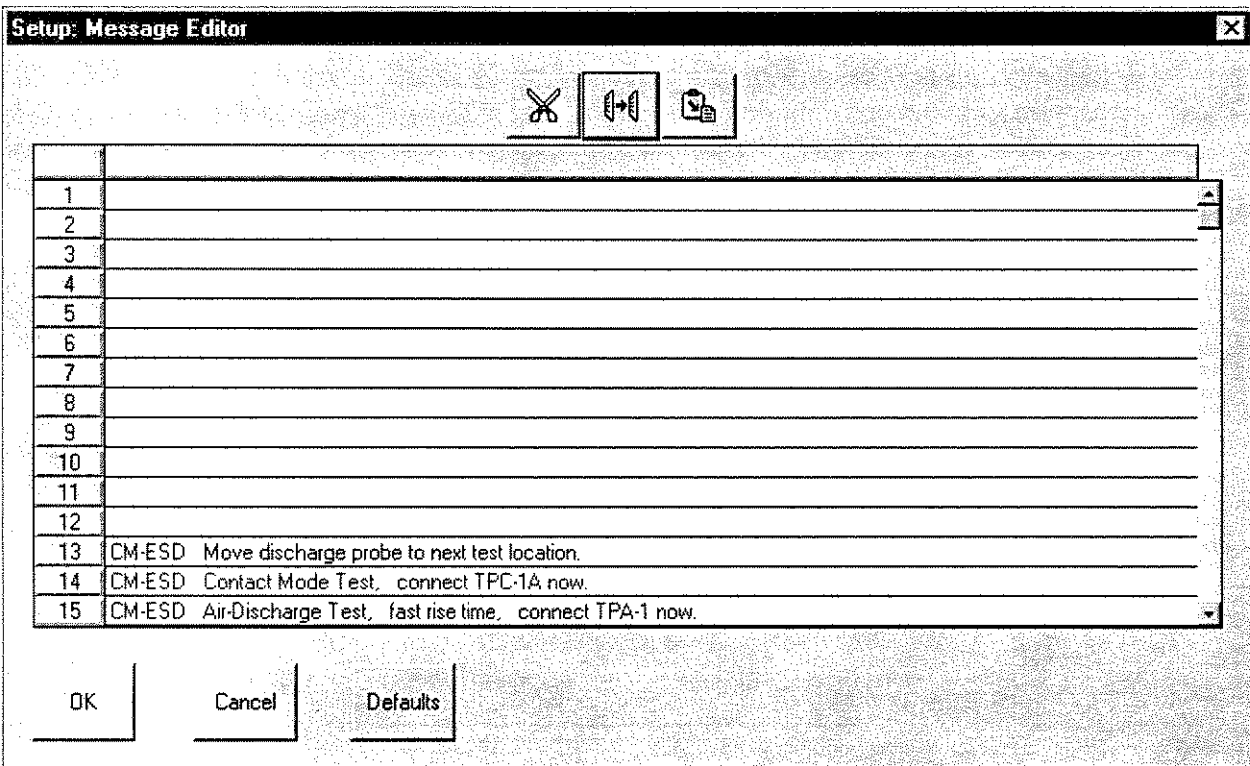

### Message Editor Screen

- Show Versions


Show Versions is a display of the version number of the **CEWare** application, plus the version of all major software components the **CEWare** application uses. When communicating remotely with an **EMCPro**, the firmware version plus the version of all major firmware components of the **EMCPro** are also shown.

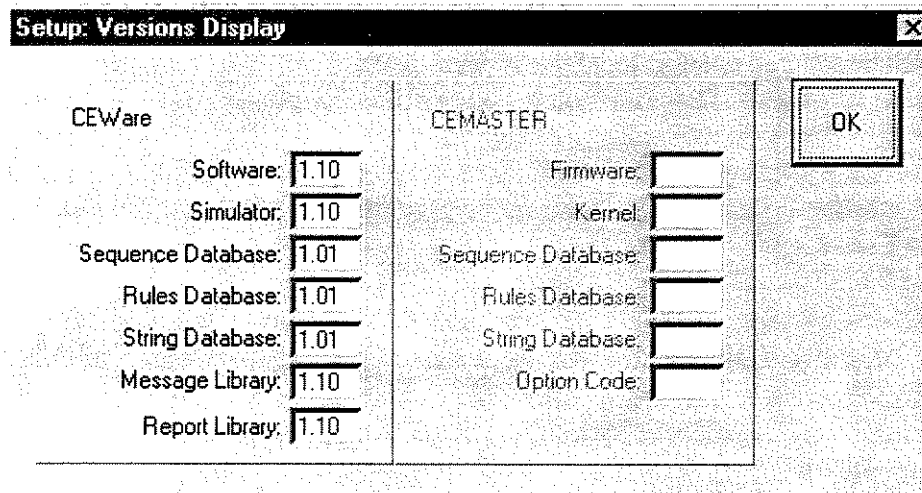

**Versions Display Screen**

- HW Selection

This selection is necessary only when running **CEWare** in local mode (with simulated hardware). The menu supports selection of test hardware type (**CEMaster** or **EMCPro**) and also of a second surge type (10/700 Telecom wave or Ring wave) if **EMCPro** is selected. Selection of this configuration information is automatic in 'Remote' mode, with hardware connected.

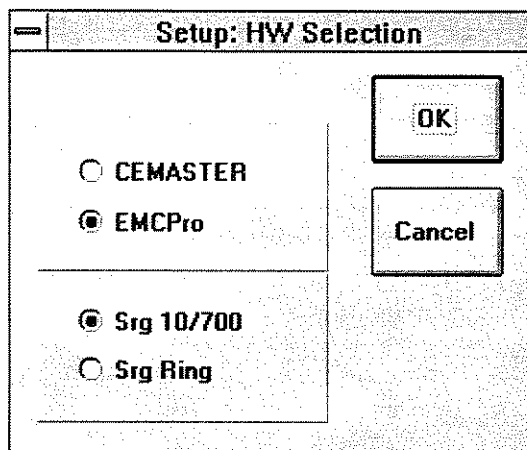

**HW Selection Screen**

Enable

There are two selections under Enable: *Remote Communications* and *Logging*. Both of these selections are ON/OFF selections that are indicated by a check mark when they are ON and no check mark when they are OFF.

- Remote Communications



---

This selection turns ON or OFF the remote (PC-based) control of the **EMCPro** by the **CEWare** application. The selection is disabled if the communications cannot be established with a **EMCPro** (communications cable not connected or **EMCPro** power is OFF). When communication with a **EMCPro** is established, this selection is enabled and **CEWare** will automatically try to turn remote control ON.

The status of communications is shown on the Status Bar at the bottom of the **CEWare** screen. When communication is not established the first item next to the “Communication:” label says DISCONNECTED. When communication is established, the label says CONNECTED.

When remote control to a **EMCPro** is enabled successfully (Remote Communications ON), the second item next to the “Communication:” label says REMOTE. When remote control is disabled (Remote Communications OFF), the item says LOCAL.

- **Logging**

This selection turns ON or OFF the logging feature for producing run time log reports. At least one of the two Log report types must have been enabled in Setup | Log Reports to enable logging or an error message will appear when you try to enable it. Logging may only be set ON or OFF when the Main Screen is visible: *Logging may not be turned ON or OFF once a run is started.*

The status of Logging is also shown on the Status Bar at the bottom of the **CEWare** screen. When Logging is not enabled the item next to the “Logging:” label says OFF. When Logging is enabled, the item says ON.

### System

These are debugging and field service functions which are not accessible by the user.

### Help

The Help menu brings up the Help file and shows the About box.

### **Toolbar**



### **Toolbar**

The toolbar holds icons for common tasks, allowing you to select that task with a single mouse-click.

- 
- File Icons -- The file icons create a new test sequence, load an existing test sequence, or save the current test sequence. If you attempt to create a new sequence or load an existing sequence, you will be prompted to save any existing work.
  - Edit Icons -- The CUT, COPY, and PASTE icons allow you to edit the test sequence grid. These icons are also found in the Sequence Editor.
  - The Printer icon will print the present sequence list, i.e. it is the same as the File | Print Sequence selection on the menu bar.

## Status Bar

The status bar at the bottom of the screen gives a quick synopsis of the **EMCPro** and test status. In some cases, the status bar will be replaced with help prompts. It contains the following information.



### System Status Bar

#### Communication

- DISCONNECTED/CONNECTED

Indicates if an **EMCPro** has been detected (CONNECTED) or not (DISCONNECTED).

- LOCAL/REMOTE

When communications with the **EMCPro** are established, this indicates whether control is from the front panel (LOCAL) or from the PC (REMOTE). The program will

---

## Communication

- DISCONNECTED/CONNECTED

Indicates if an **EMCPro** has been detected (CONNECTED) or not (DISCONNECTED).

- LOCAL/REMOTE

When communications with the **EMCPro** are established, this indicates whether control is from the front panel (LOCAL) or from the PC (REMOTE). The program will automatically go Remote; select from the menu bar (Enable | Remote Communications) to change to simulation mode when an **EMCPro** is connected and powered on.

## Run State

Shows the operating state of the **EMCPro**.

- CHARGING            Generating high voltage.
- WAITING            Between active test states, waiting for the next.
- FIRING             Generating an output.
- IDLE                No tests are running.
- RUNNING            Generating a continuous test state (EFT, ESD, or PFMF).

## Logging

Indicates if run time test information is being written to disk (ON) or not (OFF).

---

**This page intentionally left blank.**

---

# Maintenance

## Service and Maintenance Issues

There are no user serviceable parts within the **EMCPro**. Service is solely by KeyTek-trained, authorized technicians.

## Annual Calibration

Periodic calibration of the **EMCPro** is required. The recommended calibration interval is dependent on use. If periodic waveform verification is performed, calibration need be performed only if the waveform verification fails; if periodic waveform verification is not performed the recommended calibration interval is one year. Factory calibration is available; consult factory for terms and conditions.

## Factory Inspection and Refurbishment

Factory Inspection and Refurbishment is available. Consult factory for terms and conditions.

## Updating Firmware

There may be periodic updates of the **EMCPro** firmware or application software. Each update is provided with instructions for installation and use. An update of the **EMCPro** firmware requires the **PRO-SW** option be installed. If this option is not installed a KeyTek authorized service representative is required to upgrade the firmware in the field.

If you have questions about what is the latest version of firmware, contact Customer Service.

## Upgrading Hardware Options

Most hardware options can be added in the field by a KeyTek authorized service representative. Consult factory for terms and conditions.

## Decommission Issues

When decommissioning **EMCPro** equipment, the following precaution must be taken:

The **EMCPro** contains mercury relays. While the material is contained and there is no hazard in normal operation, local laws may require special consideration in disposal. Consult the factory for identification of the relays and recommendations for disposal.

---

# Troubleshooting

This section aids in finding and solving any problems you may experience. As a first step, the **EMCPro** includes diagnostic tools, accessed through the **System Menu**, and described below.

## System Menu

The System Menu gives access to several useful functions to aid in troubleshooting.

```
| SYSTEM SETUP | EUT OFF |
1. Parameters
2. Access Code
3. Diagnostics
4. Versions

|| || || || ↑ || ↓ || EXIT
```

The System menu selects special system operations; move the highlight bar using the arrow function keys and press ENTER, or press the number key associated with the sub-menu.

The **Parameters Menu** offers control of a number of system parameters, allowing customization of the **EMCPro** system. Check the menu for options available in your system; possible options are: control of the beeper; default coil factor to use; etc.

The **Access Code Menu** is not available at this time. In the future, this menu will allow locking features of the **EMCPro** system -- preventing unauthorized use.

The **Versions Menu** shows internal revisions for the code and databases used by the **EMCPro**. This information is important and should be checked whenever contacting Customer Service.

```
| VERSIONS | EUT OFF |
Firmware ..... Vx.xx
Kernel ..... Vx.xx
Sequence Database .... Vx.xx Sep 24, 96
Rule Database .... Vx.xx 16:15
String Database .... Vx.xx
Option Code .... AA
|| || || || || || EXIT
```

The Version Menu shows a Build date and time, five arguments with revisions, and a code indicating the installed options.

---

The **Diagnostics Menu** performs a quick check of basic **EMCPro** functions, and can often localize a problem and allow a field service repair rather than a factory repair.

```
|DIAGNOSTICS:TESTS | |||||EUT OFF|
1. Line Sync 1      5. ESD
2. Line Sync 2      6. RELAY
3. High Volt
4. Coil

||  ||  ||  ||  ↑  ||  ↓  ||EXIT
```

The **DIAGNOSTICS: TESTS** menu selects special system operations. Move the highlight bar using the arrow function keys and press **ENTER**, or press the number key associated with the test.

### WARNING!

---

Before running any diagnostic, remove all connections from the front panel **EUT** connector, the coaxial connector, and the safety socket connectors.

---

To use the diagnostic tests, follow the requirements from the list below, choose a test, and follow any on-screen directions. If the test halts, record any message displayed and report the message to Customer Service.

The basic functions tested are listed below:

1. **Line Sync 1** -- General Purpose check of Mains circuitry. Checks that Mains contactor is operational, thermal breaker is operational, basic wiring is OK, and line sync is operational.

*Requires: EUT Mains present, EUT Switch ON, no EUT connected, no interlock fault.*

2. **Line Sync 2** -- Checks PQF circuitry. Checks PQF transformer and contactors are operational, PQF switches are operational, and Aux line sync circuit is operational.

*Requires: EUT Mains present, EUT Switch ON, no EUT connected, no interlock fault.*

3. **High Volt** -- Checks high-voltage supply, energy storage capacitors, and discharge circuitry.

4. **Coil** -- Checks power frequency magnetic field circuitry.

*Requires: no front-panel connections, no EUT AC present, no interlock fault.*

5. **ESD** -- Checks ESD head interface circuitry.

*Requires: an ESD head, no interlock fault.*

6. **RELAY** -- Checks all internal relays and switching circuits.

*Requires: EUT Mains present, EUT switch ON, no EUT connected, no interlock fault.*

---

## Troubleshooting Guide

In the event of a problem with the **EMCPro** please follow the procedure below.

- Verify that you have properly selected all test parameters.
- Check that the **EMCPro** is properly connected to the AC Mains.
- Check that the EUT is properly connected to the **EMCPro**.
- Check all interconnections for loose connections.
- Try cycling power to the EUT and the **EMCPro**.
- Run Diagnostics tests from the System Menu.
- Contact Customer Service for guidance.



---

## Error Messages

The following are possible error messages, their causes, and possible solutions.

### **No AC Phase Reference Detected Check EUT Power switch and EUT power**

The Surge parameters specify line sync, and no AC line was detected for synchronization.

To surge without the AC mains present, change the line sync setting from "L1" to "RND" -- random.

To surge with AC mains, check that EUT power cord is plugged in, EUT power is present, and the **EMCPro** EUT switch is on; check that EUT ON is shown on the front panel display.

**NOTE:** The minimum EUT inlet voltage for dependable line synchronization is 50Vac; operation below this value may cause this error message.

### **AC Required At Mains Output Check EUT Power switch and EUT power**

During a PQF test, AC was not present (PQF requires AC to be present).

Check that EUT power cord is plugged in, EUT power is present, and the **EMCPro** EUT switch is on; check that EUT ON is shown on the front panel display.

**NOTE:** The minimum EUT inlet voltage for dependable line synchronization is 50Vac; operation below this value may cause this error message.

### **ESD Simulator Not Connected**

An ESD test is selected, and no ESD simulator head was attached.

Attach an ESD head; check that the cable is properly connected (remove ground-return cable; if the ground-return indicator does not light on the head, there is a poor connection).

### **Interlock Open Fault Power PCB Interlock**

This fault indicates a problem with an internal subsystem and requires factory service. Consult the factory for further information.

---

**Interlock Open Fault  
External Interlock**

The external interlock is open, forcing the **EMCPro** into a safe state.

If a cable is in the interlock connector, remove it and check that the fault goes away. Repair any break in the external interlock circuit.

**Mains Fault: Disconnect and check EUT  
If fault recurs contact KeyTek Service**

During a PQF test a high-current was detected, possibly due to a short in the EUT.

Disconnect the EUT and check it for possible shorts line-to-line or line-to-chassis. Retest. Test with a second EUT if possible.

If this message persists factory service is required. Consult Customer Service for detail.

**Stop Test Input Active  
Reset this Input before continuing test**

A short to ground was detected on the front panel coax, STOP TEST. Remove the short and press the EXIT button beneath the display to clear the message.

**Tilt Switch Fault  
Unit must be horizontal for test**

The **EMCPro** is orientation-sensitive and will only perform Surge and EFT testing in a horizontal position. Restore the **EMCPro** to a horizontal position and press the EXIT button beneath the display to clear the message.

**EUT Overload Fault  
Allow Time for breaker to Reset**

The **EMCPro** detected an overcurrent condition on the EUT mains output, removed mains power, and displayed this message. Press the EXIT button beneath the display to clear the message. The overcurrent detector within the **EMCPro** will reset automatically, but may take several minutes to reset. During this time you can perform other testing, but will be unable to switch the EUT power on.

---

**Timeout on Remote Control: check PC application and connection**

The **EMCPro**, while running under control of a PC, lost communications with the PC. For safety, a loss of communications halts all tests. Check connections between the PC and the **EMCPro**, and check that the PC application is running.

**Unspecified Fault  
#<fault number>**

Record the fault number and retry the failed test. If this fault persists, report it to Customer Service.

**Filing a Problem Report**

When reporting a problem to KeyTek Customer Service, please include the serial number and model number from the rear panel of the **EMCPro** (and serial number of the ESD probe or other accessories, if applicable).

If your **EMCPro** is operational, access the SYSTEM menu, VERSIONS screen and copy all the information shown to include in your trouble report.

```
| VERSIONS          |||||||||||||||EUT OFF|
Firmware           ..... Vx.xx
Kernel             ..... Vx.xx
String Database    .... Vx.xx
Option Code        .... AA
Serial Number
||  ||  ||  ||  ||  ||  ||EXIT
```

The Version Menu shows a Build date and time, five arguments with revisions, and a code indicating the installed options.

Mail, Fax, or Phone your problem report to:

**Customer Service**  
**KeyTek**  
One Lowell Research Center  
Lowell, MA 01852-4345 USA  
Voice: 978-275-0800 FAX: 978-275-0850  
E-mail: sales@keytek.com  
Web: www.thermovoltek.com

or your local, authorized service representative.



# KeyTek EMC Immunity Test System

## SELECTOR GUIDE

Standards	Test Purpose & Description	MiniZap®	CEMASTER®	EMCPro™	ECAT®	G-STRIP™
IEC 1000-4-2 Electrostatic Discharge	Requirements for simulating human ESD. Contact mode preferred for direct ESD; contact mode only for indirect ESD	15kV air 8.8kV contact	8.8kV air 4.4kV contact	8.8kV air 4.4kV contact	15kV air 8kV contact	*
IEC 1000-4-3	Radio frequency radiated immunity test (Pre-Compliance)	*	*	*	*	100kHz to 1GHz
IEC 1000-4-4 Electrical Fast Transients	Requirements for simulating "sanitized" showering arc, on both power and I/O (data and signal) lines	*	2.5kV	4.4kV	8kV	*
IEC 1000-4-5 ANSI C62.41 Surge 1.2/50µs, 8/20µs Combination Wave Category B	Requirements for simulating surges on both power and I/O (data and signal) lines	*	2.5kV	6kV	22kV	*
IEC 1000-4-5 Surge 10/700µs Telecom Wave	Requirements for simulating surges on telecommunication lines	*	*	6.6kV	7kV	*
IEC 1000-4-6	Radio frequency conducted immunity test (compliant)	*	*	*	*	IEC levels 1, 2 & 3 to 10V
IEC 1000-4-8 Power Frequency Magnetic Fields	Magnetic fields generated by AC power mains	*	30A/m	30A/m	*	*
IEC 1000-4-9 Pulse Magnetic Fields	Simulates pulsed fields found in power stations, substations and other environments where very high transients occur	*	800A/m	1000A/m	> 1000A/m	*
IEC 1000-4-11 Dips and Interrupts	Simulates voltage fluctuations of the mains	*	70%, 40%, 0% short and open	70%, 40%, 0% short and open	150%, 120%, Dips 110%, 100%, 90%, 80%, 70%, 40%, 0% short and open	*
ANSI C62.41 Surge Ring Wave Category A, B	Requirements for simulating 100kHz ring wave	*	*	6.6kV	6.6kV	*
EN55011, EN55022, EN55014, FCC Part 15	Radio frequency radiated emissions testing (pre-compliance)	*	*	*	*	100kHz to 1GHz
CCITT Rec. K.17, K.20, K.21 Surge 10/700µs Telecom Wave	For qualifying telecom repeaters, central office and station (i.e., subscriber) equipment	*	*	6.6kV	7kV	*
UL 1449 Surge Combination Waves	Qualification tests for AC powerline protectors. Three levels of 6kV combination wave required: 3kA, 750A and 500A	*	*	3kA	3kA, 750A, 500A	*
FCC Part 68 Telecom	For qualifying telecom equipment: specifies surge tests on telecom lines	*	*	9/720µs waveform, 1000V only	9/720µs waveform, 1000V; 10/160µs waveform, 1500V; 10/360µs waveform, 800V	*
FCC Part 68 Power Lines	For qualifying telecom equipment: specifies surge tests on power lines	*	*	*	2/10µs waveform, 2500V	*
GR-1089-CORE Bellcore	Surge test requirements for telecom equipment installed in various locations	*	*	*	2/10µs waveform, 800V, 1500V, 5000V (AC mains)  10/360µs waveform 1000V  10/1000µs waveform 600V, 1000V, 1500V	*

\* Not applicable



# KeyTek Application Note

## Dips and Interrupts Testing per IEC 1000-4-11

### DIPS AND INTERRUPTS BACKGROUND

---

Dips and interrupts can occur on the AC power mains as a result of a fault in the distribution system such as an open circuit breaker or a sudden large load being turned on in the immediate vicinity. A power distribution system fault can cause a switch in the distribution grid to open and close a number of times, resulting in multiple interrupts to electrical and electronic equipment.

Electronic products are tested for immunity to dips and interrupts to insure their continued reliable operation if subjected to dips and/or interrupts on the AC power mains. The European Union's EMC Directive mandates dips and interrupts testing for virtually all electrical and electronic products as a condition for obtaining the CE Mark before shipping products to member states of the European Union.

### APPLICABLE STANDARDS

---

Generic Immunity Standards, Product Standards and Product Family Standards require that dip and interrupt tests be performed in accordance with Basic EMC Standards: IEC 1000-4-11 and EN 61000-4-11<sup>1</sup>. KeyTek's Application Note, "EMC Standards

<sup>1</sup> IEC 1000-4-11 and EN 61000-4-11 are virtually identical standards.

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD

---

The Basic EMC Standard for Dips and Interrupts defines methods of generating consistently reproducible electrical dips and interrupts for test purposes. They specify characteristics of the AC mains to the EUT such as peak inrush current, transition times and durations.

While the Basic EMC Standard specifies how to perform Dips and Interrupts testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail Performance Criteria.

### TEST LEVELS

---

Standard	Applicability	Levels
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	Not required
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	0%, 40%, 70% & 100%
EN 50082-2	Generic Immunity - Industrial Environment	Not required
EN 50082-2 Draft	Generic Immunity - Industrial Environment	0%, 40%, 70% & 100%
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	0%, 40%, 70% & 100%





# Dips and Interrupts Testing per IEC 1000-4-11


## PEAK INRUSH CURRENT

IEC 1000-4-11 requires the simulator be capable of supplying peak inrush currents of up to 500A for 220V to 240V mains, and up to 250A for 100V to 120V mains. Additionally, the Standard requires this capability be measured using a bridge rectifier connected via a switch to a discharged 1700 $\mu$ F capacitor. The parallel discharge resistance should be chosen to allow several RC time constants between tests. An example in Annex A (normative) uses a 10k ohm resistance, providing a time constant of 17 s, "...so that a wait of 1.5 to 2 minutes should be used between inrush drive capability tests."

The test for inrush current is performed by switching the generator from 0% to 100% at both 90° and 270° to insure sufficient peak inrush current drive capability for both polarities.

## WAVEFORM VERIFICATION

IEC 1000-4-11 requires that the simulator output be verified periodically. For Dip and Interrupt test simulators, it is necessary to verify the voltage transition levels, transition times to 100%, and the inrush current capability. Most modern oscilloscopes are capable of observing the voltage levels and transition times. For verifying the inrush current, a bridge rectifier, suitably rated 1700 $\mu$ F capacitor and appropriate current transformer are required.

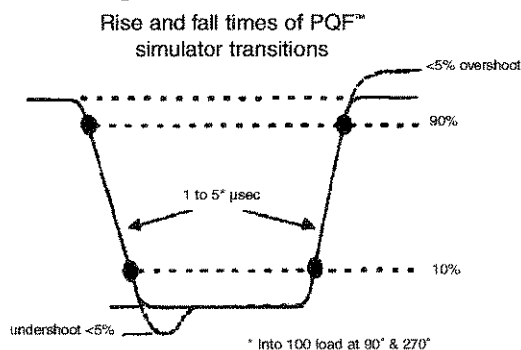

## TEST EXECUTION

According to IEC 1000-4-11, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- Input power of the EUT
- Performance Criteria
- Operation modes of the EUT
- Test set-up description
- Type of designation of the EUT
- Information on possible connections, cables, peripherals, etc.

After each group of tests, a complete functional test must be performed.

## EUT PERFORMANCE CRITERIA

For Dip and Interrupt tests, Performance Criteria varies in some standards depending on the duration or severity of the dip and/or interrupt. Under some conditions, loss of function is allowed, provided that the function is self-recoverable or can be restored by the control operations. Under less severe conditions, degradation of performance is allowed during the test, however, the unit must continue to operate as intended after the test. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## DIP AND INTERRUPT SIMULATORS

Dip and Interrupt Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-11, including those for peak inrush current. Additionally, KeyTek simulators meet the fast switching time requirements not only to 100% as required by the standards, but from any level to any other level. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark and PQF is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice.  
Printed in USA. 10/97



# KeyTek Application Note

## Pulse Magnetic field Testing per IEC 1000-4-9

### PULSE MAGNETIC FIELD BACKGROUND

Pulse Magnetic Fields are produced as a result of a large current impulse through a conductor. An example is lightning current flowing through a grounding conductor at a power sub-station. Pulse magnetic fields can also occur in heavy industrial areas where very large current impulses are used in a manufacturing process.

Electronic products are tested for immunity pulse magnetic fields to insure their continued reliable

operation when placed in service in a very harsh environment. Although most electrical and electronic products will not have to be tested for pulse magnetic field immunity, the European Union's EMC Directive may mandate this testing as a condition for obtaining the CE Mark under special circumstances and for specific products before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Although not currently required by Generic Immunity, Product specific, or Product Family Standards, future standards may require Pulse Magnetic Field tests be performed in accordance with Basic EMC Standards: IEC 1000-4-9 and EN 61000-4-9<sup>1</sup>. KeyTek's Application

Note, "EMC Standards Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

<sup>1</sup> IEC 1000-4-9 and EN 61000-4-9 are virtually identical standards.

### BASIC EMC STANDARD

The Basic EMC Standard for Pulse Magnetic Field defines methods of generating consistently reproducible current impulses for test purposes. Field amplitudes required by these standards range from

100 - 1000 Amps per meter. Although applicable only to apparatus containing devices susceptible to magnetic fields, testing may be required to make that determination.

### TEST LEVELS

Installation Environment	IEC 1000-4-9 Level	Field Strength A/m
Environment where sensitive devices using electron beams can be used	1	N/A
Residential, office and hospital areas far away from earth conductors of lightning protection systems	2	N/A
Commercial areas, control building, field of industrial plants with lightning protection system or metallic structures nearby	3	100
Heavy industrial and power plants and H.V. substation control rooms	4	300
Switchyard areas of heavy industrial plants	5	1000
Higher or lower environmental levels than those described above	X	X

### TEST SET-UP


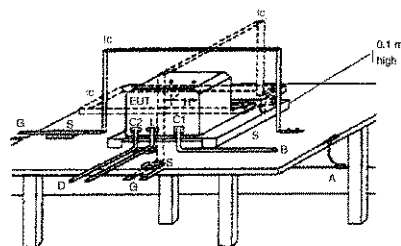


TABLE TOP SET-UP



FLOOR STANDING SET-UP

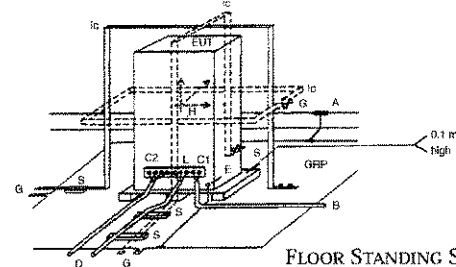


# Pulse Magnetic Field Testing per IEC 1000-4-9

## COUPLING METHODS

An Induction Coil having a standard dimension of 1 meter per side for a rectangular coil, or 1 meter diameter for a circular coil, is to be used for testing small equipment. This coil has a test volume of 0.6m x 0.6m x 0.5m (h). For floor standing equipment, larger dimensions can be used; however, the coil shall be able to envelop the EUT and the coil dimensions must give a minimum distance of coil conductors to EUT walls equal to 1/3 of the dimension of the EUT being tested.

## WAVEFORM VERIFICATION

Basic test standards require that the simulator output be verified periodically. In the case of the Pulse Magnetic Field, verification is accomplished by verifying the amplitude of the 8/20 $\mu$ s current pulse driving the coil. An appropriate current transformer (Pearson Model 110 or equivalent) and an oscilloscope with a bandwidth of >100MHz capable of displaying a single pulse are required.

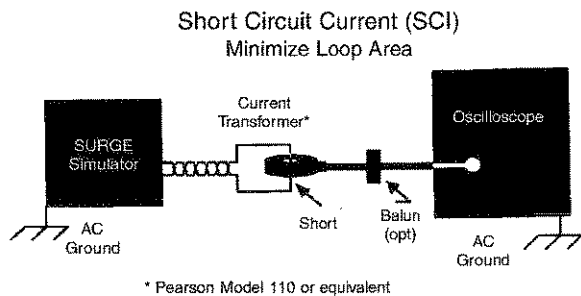

## TEST EXECUTION

According to IEC 1000-4-9, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- How the test is performed
- Verification of the laboratory reference conditions
- Preliminary verification of the correct operation of the EUT
- An evaluation of the test results

## TEST APPLICABILITY

According to Annex A of IEC 1000-4-9, test levels shall be selected in accordance with the most realistic installation and environmental conditions. Tests are recommended for equipment operating in areas characterized by proximity of conductors of lightning protection systems and or structures, or the proximity of conductors, bus-bars or medium to high voltage lines carrying tens of kA.

## PULSE MAGNETIC FIELD SIMULATORS

Pulse Magnetic Field Simulators and standard coils provided by KeyTek Instrument Corporation meet the pulse waveform and amplitude requirements for testing to >1000A/m in accordance with IEC 1000-4-9. Consult KeyTek for larger coils used for testing floor standing equipment. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97




# Pulse Magnetic Field Testing per IEC 1000-4-9

## COUPLING METHODS

An Induction Coil having a standard dimension of 1 meter per side for a rectangular coil, or 1 meter diameter for a circular coil, is to be used for testing small equipment. This coil has a test volume of 0.6m x 0.6m x 0.5m (h). For floor standing equipment, larger dimensions can be used; however, the coil shall be able to envelop the EUT and the coil dimensions must give a minimum distance of coil conductors to EUT walls equal to 1/3 of the dimension of the EUT being tested.

## WAVEFORM VERIFICATION

Basic test standards require that the simulator output be verified periodically. In the case of the Pulse Magnetic Field, verification is accomplished by verifying the amplitude of the 8/20 $\mu$ s current pulse driving the coil. An appropriate current transformer (Pearson Model 110 or equivalent) and an oscilloscope with a bandwidth of >100MHz capable of displaying a single pulse are required.

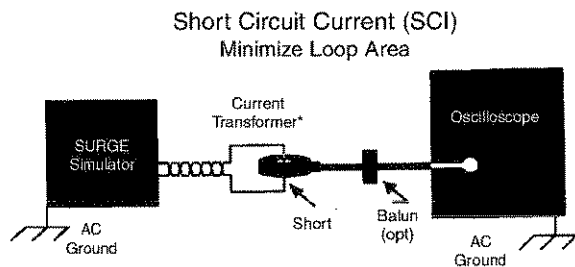

## TEST EXECUTION

According to IEC 1000-4-9, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- How the test is performed
- Verification of the laboratory reference conditions
- Preliminary verification of the correct operation of the EUT
- An evaluation of the test results

## TEST APPLICABILITY

According to Annex A of IEC 1000-4-9, test levels shall be selected in accordance with the most realistic installation and environmental conditions. Tests are recommended for equipment operating in areas characterized by proximity of conductors of lightning protection systems and or structures, or the proximity of conductors, bus-bars or medium to high voltage lines carrying tens of kA.

## PULSE MAGNETIC FIELD SIMULATORS

Pulse Magnetic Field Simulators and standard coils provided by KeyTek Instrument Corporation meet the pulse waveform and amplitude requirements for testing to >1000A/m in accordance with IEC 1000-4-9. Consult KeyTek for larger coils used for testing floor standing equipment. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97





# KeyTek Application Note

## Power Frequency Magnetic Field Testing per IEC 1000-4-8

### POWER FREQUENCY MAGNETIC FIELD BACKGROUND

Electronic products are often subjected to magnetic fields at AC mains frequencies. These fields are frequently produced in the vicinity of power transformers and can cause problems with video displays, Hall effect sensors, and other electronic products having a sensitivity to magnetic fields. Electronic Products are tested for immunity to power

frequency magnetic fields to insure their continued reliable operation when placed in service. The European Union's EMC Directive currently mandates power frequency magnetic field testing for certain categories of equipment as a condition for obtaining the CE Mark before shipping products to member states of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require that Power Frequency Magnetic Field tests be performed in accordance with Basic EMC Standards: IEC 1000-4-8 and EN 61000-4-8'. KeyTek's Application Note, "EMC Standards

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and list sources for procuring copyrighted documents.

### BASIC EMC STANDARD

The Basic EMC Standard for Power Frequency Magnetic Field defines methods of generating consistently reproducible magnetic fields for test purposes. Although higher magnetic field levels are described, compliance to the Generic Immunity Standard for residential and commercial products is 1A/m or 3A/m. Currently applicable only to apparatus

containing devices susceptible to magnetic fields, testing of other products may be required to make that determination. While the Basic EMC Standard specifies how to perform Power Frequency Magnetic Field testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Power Frequency Magnetic Field testing is required for products that could be affected by magnetic fields, including CRTs and Hall Effect Sensors and is strongly recommended for all products.

Standard	Applicability	Magnetic Field Level
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	Not required
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	3A/m
EN 50082-2	Generic Immunity - Industrial Environment	30A/m
EN 50082-2 Draft	Generic Immunity - Industrial Environment	30A/m
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	Not required

### TEST SET-UP


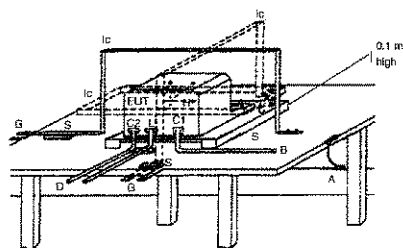


TABLE TOP SET-UP



FLOOR STANDING SET-UP

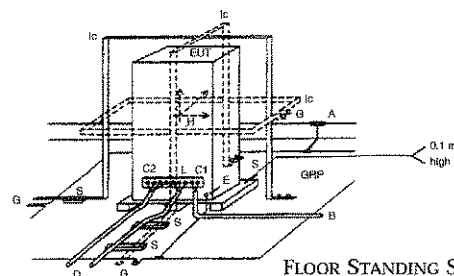

# Power Frequency Magnetic Field Testing per IEC 1000-4-8

## COUPLING METHODS


An Induction Coil having standard dimensions of 1 meter per side for a rectangular coil, or 1 meter diameter for a circular coil, is to be used for testing small equipment. For large equipment, larger dimensions may be used; however, the coil shall be able to envelop the EUT and the coil dimensions must give a minimum distance of coil conductors to EUT walls equal to 1/3 of the dimension of the EUT being tested.

## WAVEFORMS



## WAVEFORM VERIFICATION

IEC 1000-4-8 requires that the simulator output and magnetic field be verified periodically. Any oscilloscope is capable of verifying the power frequency AC current to the coil. Monitoring the actual field requires an AC field probe and monitor, such as the CM-HMON available from KeyTek.

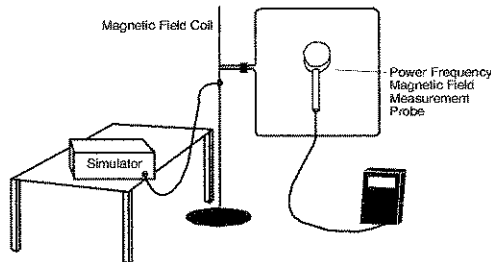

## TEST EXECUTION

According to IEC 1000-4-8, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- How the test is carried out
- Verification of the laboratory reference conditions
- Preliminary verification of the correct operation of the EUT
- An evaluation of the test results

## EUT PERFORMANCE CRITERIA

For Power Frequency Magnetic Field tests, the Generic Immunity Standards require that the product continue to operate as intended during the test, however, CRT interference is allowed above 1A/m in the residential, commercial and light industrial draft standard, and above 3A/m in the industrial standard. No degradation or loss of function is allowed below a performance level specified by the manufacturer. The performance level may be replaced by a permissible loss of performance. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## POWER FREQUENCY MAGNETIC FIELD SIMULATORS

Power Frequency Magnetic Field Simulators and standard coils provided by KeyTek Instrument Corporation meet all the minimum requirements for performing tests to >3A/m in compliance with the applicable Generic and Product Family Standards.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97



# KeyTek Application Note

## Surge Testing per IEC 1000-4-5

### SURGE BACKGROUND

Surges occur on the AC power mains as a result of switching operations in the power grid and from nearby lightning strikes, either directly to the power distribution system or to nearby ground. Radiated coupling of surges into I/O lines generally occurs only when the lines are very long.

Electronic products are tested for Surge immunity to insure their continued reliable operation if subjected to

realistic levels of surge voltages. The European Union's EMC Directive currently mandates Surge testing for some products; however, it is expected that virtually all electrical and electronic products will have to be tested for Surge immunity in the near future as a condition for obtaining the CE Mark before shipping products to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require Surge tests be performed in accordance with Basic EMC Standards: IEC 801-5, IEC 1000-4-5 or EN 61000-4-5. KeyTek's Application Note, "EMC Standards Overview," provides an overview

of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD

The Basic EMC Standard for Surge defines the methods of generating consistently reproducible surge voltages for test purposes. They specify generator and coupler/decoupler design and performance in sufficient detail to produce correlatable results between test sites.


While the Basic EMC Standard specifies how to perform Surge testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Standard	Applicability	Common Mode	Differential Mode
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	N/A	N/A
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	2kV	1kV
EN 50082-2	Generic Immunity - Industrial Environment	N/A	N/A
EN 50082-2 Draft	Generic Immunity - Industrial Environment	4kV	2kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	2kV	1kV

### SAFETY

When performing Surge tests, safety is a primary concern. Surge voltages and currents must be contained to insure they will not appear where they can cause damage to other instruments in the test area. The test pulses used for Surge testing are of sufficient energy to cause components to fragment under fault conditions and become hazardous to personnel in unprotected environments.

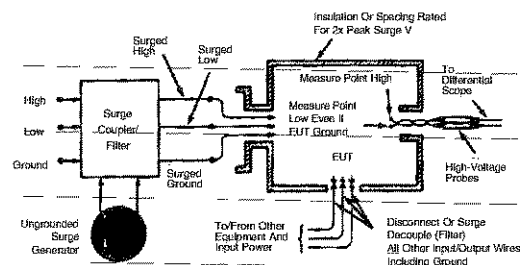




# Surge Testing per IEC 1000-4-5

## COUPLING METHODS

**Capacitive Coupling** via 9 $\mu$ F (Line to earth) or 18 $\mu$ F (line to line) capacitors is required for coupling surges to AC or DC power mains. These coupling capacitors are typically included as part of a Coupler/Decoupler (C/D) in commercially available Surge simulators. The C/D provides both coupling to the EUT power mains and a decoupler to prevent the surge from appearing on the ac mains connected to other equipment in the lab.


**Capacitive Coupling** via .5 $\mu$ F capacitors, as well as via alternative devices such as surge arrestors, are used to couple surges onto data, I/O and telecommunication lines. Surge arrestors are the preferred coupler device due to the undesirable loading effects of capacitors particularly at frequencies greater than a few kilohertz. A decoupler is included to prevent the surge from appearing at, and potentially damaging, the auxiliary equipment.

## WAVEFORMS

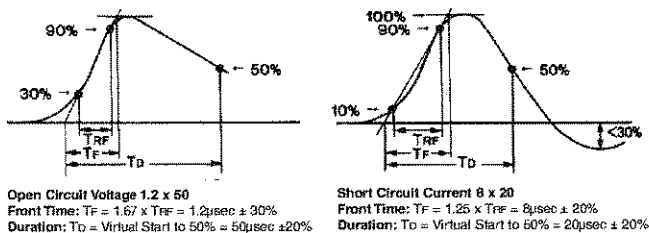

## WAVEFORM VERIFICATION

IEC 1000-4-5 requires that the simulator output be verified periodically. High voltage differential surge probes are required for verifying the open-circuit voltage, and a suitable current transformer (Pearson Model 110 or equivalent) is required for verification of the short-circuit current. A digital or storage oscilloscope with 100MHz bandwidth is sufficient for measuring the surge voltage and current waveforms and peaks.

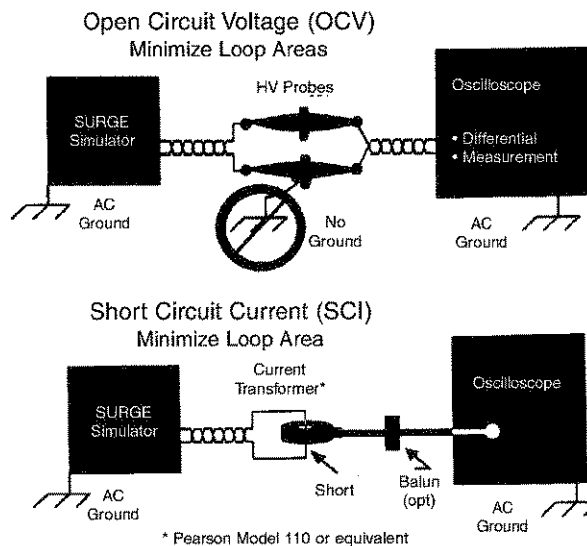

## TEST EXECUTION

According to IEC 1000-4-5, testing must be carried out according to the manufacturer's test plan, which shall specify:

- Generator & other equipment
- Generator Source Impedance
- Repetition rate (one per minute maximum)
- Sequence of application of the surge
- Installation conditions
- Operating conditions of EUT
- Number of tests (at least five positive and five negative at each point)
- Test levels
- Polarity
- Inputs/outputs tested
- Phase angle of coupling to ac mains
- Internal or external trigger

## EUT PERFORMANCE CRITERIA

For Surge tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating status or data storage. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## SURGE SIMULATORS

Surge Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-5, including dynamic source impedance, all waveform characteristics, and coupler/decoupler design. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97





# KeyTek Application Note

## EFT Testing per IEC 1000-4-4

### EFT BACKGROUND

Electrical Fast Transients (EFT) are caused anytime a gaseous discharge occurs (a spark in air or other gas), the most common being the opening of a switch through which current is flowing. As the switch is opened, arcing occurs between the contacts; first at a low voltage and high frequency while contacts are close together, and later at a higher voltage and lower frequency as the contacts become separated. Coupling of the EFT into electronic products occurs when power cables handling

high currents are run in close proximity to power, data, and/or I/O cables.

Electronic products are tested for EFT immunity to insure their continued reliable operation if subjected to realistic levels of fast transients. The European Union's EMC Directive mandates EFT testing for virtually all electrical and electronic products as a condition for obtaining the CE Mark before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require that EFT tests be performed in accordance with Basic EMC Standards: IEC 801-4, IEC 1000-4-4 or EN 61000-4-4<sup>1</sup>. KeyTek's Application Note,

"EMC Standards Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

<sup>1</sup> IEC 801-4, IEC 1000-4-4, and EN 61000-4-4 are essentially the same for test voltages and levels.

### BASIC EMC STANDARD



The Basic EMC Standards for EFT define methods of generating consistently reproducible fast transients for test purposes. They specify generator and coupler/decoupler design and performance in an attempt to produce correlational results between test sites. The

Basic EMC Standard specifies how to perform EFT testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Standard	Applicability	Test Voltage
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	1kV
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	1kV
EN 50082-2	Generic Immunity - Industrial Environment	2kV
EN 50082-2 Draft	Generic Immunity - Industrial Environment	2kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	1kV

### TEST SET-UP

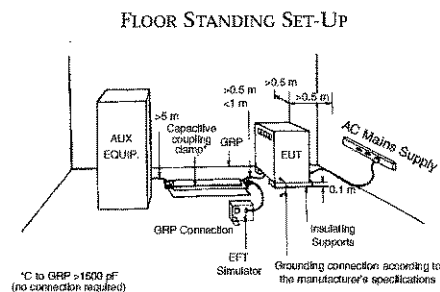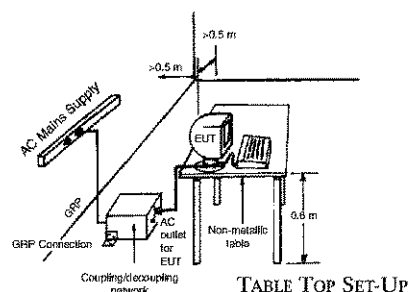



# EFT Testing per IEC 1000-4-4


## COUPLING METHODS

**Capacitive Coupling** via 33nF capacitors is the required coupling method to AC or DC power mains. These coupling capacitors are included as part of a Coupler/ Decoupler (C/D) in commercially available EFT simulators. The design of the decoupling portion of the C/D, which prevents the EFT burst from traveling back onto the power mains, is also specified in IEC 1000-4-4.

A **Capacitive Coupling Clamp** is used to couple EFT bursts onto data, I/O, and telecommunications lines. Construction of the clamp is shown in Figure 5 of IEC 1000-4-4; however, considerable differences exist in commercially available clamps. Some clamps use higher quality materials and some designs allow for the use of an optional safety interlocked cover.

## WAVEFORMS

### STANDARD EFT WAVEFORM

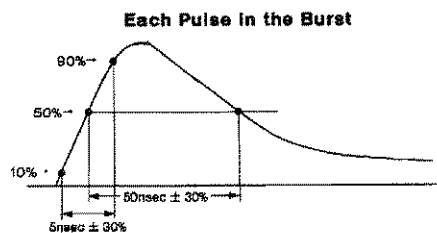

## WAVEFORM VERIFICATION

IEC 1000-4-4 requires that the simulator output be verified periodically. A 50 ohm load and attenuator rated for high voltage is required and the measurement must be made using an oscilloscope with at least 400MHz bandwidth.

One problem noted with IEC 1000-4-4 is that simulator designs can be quite different and although each has a 50 ohm source impedance and provides the specified pulse into a 50 ohm termination, some simulators provide significantly more or less energy than others into loads that are not 50 ohms - the AC power input of most electronic products is something other than 50 ohms. To deal with the problems, changes to the standard were proposed to require waveforms be verified into a 1000 ohm load. Unfortunately, these changes were not accepted; however, this and other proposed improvements to IEC 1000-4-4 will be included in a forthcoming Annex.

## TEST EXECUTION

According to IEC 1000-4-4, testing must be carried out according to the manufacturer's test plan, which shall specify:

<b>Type of test</b>	Test levels
<b>Polarity (+ &amp; - required)</b>	Test duration (1 minute minimum)
<b>Number of Voltage tests</b>	EUT ports
<b>EUT operating condition</b>	Sequence to tests to ports, etc.
<b>Auxiliary equipment</b>	

## EUT PERFORMANCE CRITERIA

For EFT tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating status or data storage. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## EFT SIMULATORS

EFT Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-4, including discharge pulse energy, output type, dynamic source impedance, and all waveform characteristics. Additionally, KeyTek simulators meet the requirements for coupling/decoupling networks for AC and DC mains as described in paragraph 6.2 of IEC 1000-4-4. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97



# KeyTek Application Note

## ESD Accessories for Testing Beyond IEC 1000-4-2

### REAL WORLD TESTING

ESD is the most common cause of failure in computer based equipment. It accounts for hundreds of millions of dollars in downtime and repair costs each year.

Fortunately, catastrophic failures are preventable and many manufacturers have R&D and manufacturing programs to insure that their products are ESD resistant when shipped. The European Union's EMC Directive requires that virtually all electronic and electrical products be tested for a minimum level of ESD immunity.

### APPLICABLE STANDARDS

Generic Immunity Standards, Product Standards and Product Family Standards require that ESD tests be performed in accordance with specific Basic Test Standards: IEC 801-2, IEC 1000-4-2 or EN 61000-4-2.

### BASIC EMC STANDARDS

The Basic EMC Standards for ESD define methods of generating consistently reproducible electrical stresses

### APPLYING DISCHARGES

ESD is applied both directly to the Equipment Under Test (EUT) and indirectly, via horizontal and vertical coupling planes.

Direct coupling is performed with either a contact mode discharge to metal surfaces of the EUT (preferred method), or via an air discharge. In both cases, discharges must be made to all points and surfaces accessible to personnel during normal usage. Tests are performed using 10 single discharges per test point in the most sensitive polarity.

Indirect discharges are performed to simulate radiated ESD events to the EUT. Using the vertical coupling

plane (VCP), at least 10 discharges to the center of the edge of the plane are required with the VCP positioned to completely radiate towards four faces of the EUT.

The horizontal coupling plane (HCP) is on the surface of the work table and is covered with a material to electrically insulate it from the EUT. Currently, a discharge is made to the surface of the HCP at a distance of 0.1m from each side of the EUT, however, an amendment is in process to modify this procedure and require discharges to be made to the center of the edge of the HCP.



However, experience by manufacturers has shown that the characteristics of real ESD vary somewhat from the test pulses required by mandatory standards. Current rise times are much faster and fields associated with discharges are more significant than thought.

In order to insure that products are immune to real ESD events, it is necessary to test beyond the requirements of the mandatory standards using different discharge tips, coupling planes and other accessories.

KeyTek's Application Note "EMC Standards Overview" provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

for test purposes. (Refer to ESD Testing per IEC 1000-4-2 Application Note.)

### TEST SET-UP

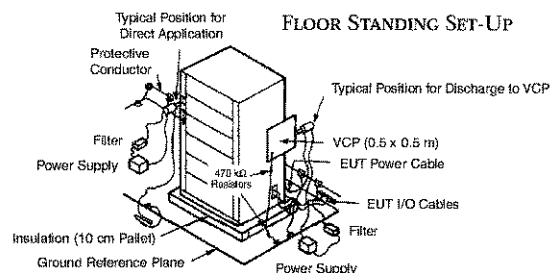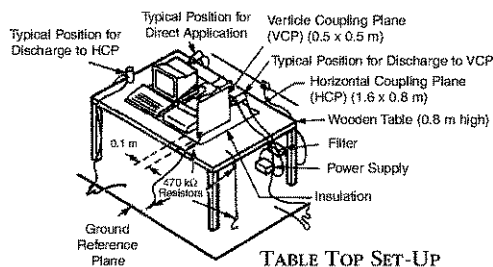



Handwritten scribbles or marks in the lower center of the page.

# ESD Accessories for Testing Beyond IEC 1000-4-2

## CM-ESD AND PRO-ESD TIPS

---

Simulator tips are included with CM-ESD and PRO-ESD for both contact mode testing (TPC-3) and air discharge testing (TPA-2) in accordance with IEC 1000-4-2. For very fast, real-world rise times, the TPA-1 for air discharge will provide rise times on the order of 0.4ns or faster.

A method used successfully for locating ESD and RF susceptibility problems is self-discharge: producing the spark associated with an air discharge, but without actually discharging to the equipment under test. This is done using the TPF-1 self-discharge tip in the vicinity of suspect cables, connectors, shields and the like.

Another useful tool is the 50-MZ standoff spacer for air-discharge testing. This allows the user to set the precise distance between the tip and the target equipment, useful for investigative work.

When trying to determine the real cause of an ESD immunity problem, it is useful to separate E-Field and H-Field effects. This is easily accomplished with the MZT-11 E-Field and MZT-12 H-Field Simulator Tip Assemblies.

In order to determine if fields are being generated and to observe the relative levels of those fields, the FCS-1 Field and Corona Sensor Group was developed.

This option includes a basic monitor unit, HEC-1, H-Field Sensor, HFS-1, E-Field Sensor, EFS-1, and Pre-discharge Corona Sensor, CCS-1.

## COUPLING PLANES

---

Two coupling planes, one horizontal and one vertical, are required for product testing in accordance with IEC 1000-4-2. The Horizontal Coupling Plane, a model HCP-1, is placed on a non-conductive table below the equipment being tested. A discharge to the HCP-1 will then cause a horizontally polarized field to be radiated up into the product being tested. A Vertical Coupling Plane, model VCP-1, is oriented at a fixed distance from the product being tested. A discharge is made to the edge of the VCP-1 causing a vertically polarized field to be radiated towards the product. All four sides of the product must be tested in this manner.

Another type of plane available as an accessory to the CM-ESD and PRO-ESD is the TP-3, a 1.5m x 1.5m Target Plane used with the CTC-3 ESD target for waveform verification. The CTC-3 is mounted in the center of the plane and the ESD current is monitored on an oscilloscope which is installed inside a Faraday cage.

## OTHER ACCESSORIES

---

In order to obtain an independent measurement of the ESD voltage on the tip of the CM-ESD and PRO-ESD, a calibrated attenuator, such as the DCA-2 is required. With the attenuator in place, the output voltage can be read using any DC attenuator.

For customers planning to ship the CM-ESD and PRO-ESD between facilities on a regular basis, the MCA-1 Hard Carrying Case is recommended. No additional shipping materials are required. Secure the unit in the MCA-1, affix the proper labels, and call the shipper.

Some corporate standards require testing with hundreds or even thousands of discharges to a point on the equipment under test. A non-conducting tripod, such as the T-2, allows the CM-ESD and PRO-ESD simulator to be held steady against the equipment being tested, without interfering with the test results.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
<http://www.keytek.com>

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 4/98





# KeyTek Application Note

## ESD Testing per IEC 1000-4-2

### ESD BACKGROUND

Electrostatic Discharge (ESD) is the abrupt release of charge from one object (often a person) to another. Such a discharge can permanently damage or otherwise upset the function of sensitive electronic circuits.

Electronic products are tested for ESD immunity to insure their continued reliable operation if subjected to

realistic levels of ESD after being placed in service. The European Union's EMC Directive mandates ESD immunity testing for virtually all electrical and/or electronic products as a condition for obtaining the CE Mark before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity Standards, Product Standards and Product Family Standards require that ESD tests be performed in accordance with specific Basic EMC Standards: IEC 801-2, IEC 1000-4-2, or EN 61000-4-2. KeyTek's Application Note, "EMC Standards

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD



The Basic EMC Standards for ESD define methods of generating consistently reproducible electrical stresses for test purposes. They specify capacitances and resistances to model the human body's charge storing capability and discharge impedance, respectively.

This model results in a current waveform, defined in the Standards. While the Basic EMC Standard also specifies how to perform ESD testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail Performance Criteria.

### TEST LEVELS

Standard	Applicability	Contact Discharge Test Voltage	Air Discharge Test Voltage
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	N/A	8kV
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	4kV	8kV
EN 50082-2	Generic Immunity - Industrial Environment	4kV	8kV
EN 50082-2 Draft	Generic Immunity - Industrial Environment	4kV	8kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	4kV	8kV

### TEST SET-UP

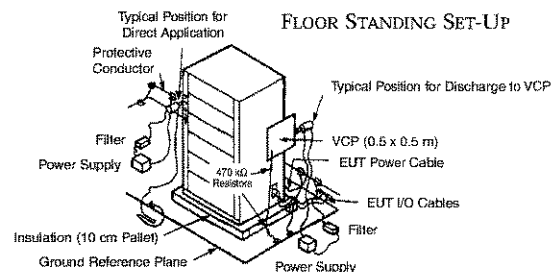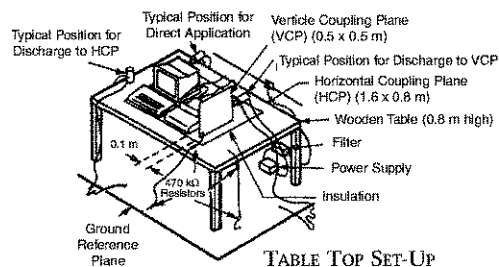




# ESD Testing per IEC 1000-4-2

## COUPLING METHODS

Direct Coupling is a discharge directly to the Equipment Under Test (EUT), either in an Air Discharge mode, necessary for products having few or no metal surfaces, or via Contact mode, the preferred method. In the "air discharge" mode, the ESD event is initiated when the test simulator output is brought into close proximity with the EUT until a spark is initiated. The resulting stress is influenced by various environmental factors. In the preferred "contact discharge" mode, the test simulator output is first brought into physical contact with the EUT, then the ESD event is initiated under controlled conditions within the simulator.

Indirect Coupling simulates an ESD event which causes a radiated field to be emitted in the vicinity of the victim equipment. This is accomplished using Vertical Coupling Planes (VCP's) and Horizontal Coupling Planes (HCP's). Current standards require discharges be made to the edge of the VCP and surface of an HCP.

## WAVEFORMS

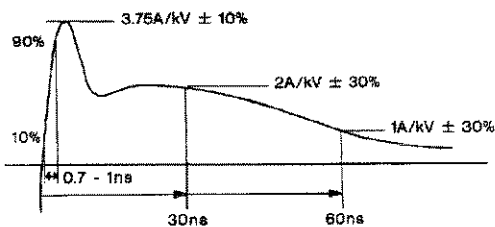

## WAVEFORM VERIFICATION

IEC 1000-4-2 requires the simulator output be verified periodically. A Model CTC-3 measurement target and target plane is required. The ESD current measurement is then made using a measurement system having a 1GHz or greater bandwidth. It is necessary to place the oscilloscope inside a shielded enclosure during the measurement to reduce the effects of radiated ESD directly to the measurement instrument.

Recent work by the Working Group 14.0 of the ESD Association has found that some simulators produce waveforms that are in compliance with IEC 1000-4-2, but have considerable ringing and high frequency components that do not show up with 1GHz instrumentation. These simulators may cause failures in products which would not occur if tested with a KeyTek simulator. Working Group 14.0 is preparing a document to describe waveform verification methods to allow manufacturers to verify the ESD current from simulators using high bandwidth instrumentation.

## NUMBER AND RATE OF DISCHARGES

The manufacturer is required to develop a test plan identifying the EUT's most sensitive operating mode and appropriate test points. A minimum of 10 discharges are then made to each test point in either Contact Discharge or Air Discharge, according to the test plan. A recommended time interval of 1 second between tests should be used, but a longer interval is allowed if necessary to determine if a system failure has occurred.

For the indirect tests, 10 discharges are required to the Vertical Coupling Plane at each of 4 equipment faces (40 discharges) and then 10 discharges are required to the Horizontal Coupling Plane at 4 sides of the EUT (40 discharges).

## EUT PERFORMANCE CRITERIA

For ESD tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating state or stored data. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## ESD SIMULATORS

ESD Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-2, including discharge network characteristics, discharge tips, and waveforms. Numerous accessories and discharge tips are available from KeyTek for those manufacturers requiring additional test capability and flexibility. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Volttek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Volttek Corporation. ©Thermo Volttek.  
Specifications are subject to change without notice. Printed in USA. 10/97



# KeyTek Application Note

## Standard Selector Guide

### PRODUCT AND PRODUCT FAMILY STANDARDS

---

As of January 1, 1996, all electrical or electronics products shipped into the European Union that could either cause electromagnetic interference (EMI) or could be susceptible to EMI, must be tested to ensure adherence to the EMC Directive. (If a manufacturer believes that a product does not cause EMI and is not affected by EMI, the onus is on the manufacturer to substantiate his claims.)

In order to comply with the EMC Directive, the following products listed must conform to applicable Product or Product Family Standards. If no Product or

Product Family Standards exist, the product must comply with the Generic Immunity and Emissions standards. These generic standards are divided into two areas:

<b>Environment</b>	<b>Generic Emissions</b>	<b>Generic Immunity</b>
Residential, commercial, and light industrial	EN 50081-1	EN 50082-1
Industrial	EN 50081-2	EN 50082-2

### RESIDENTIAL, COMMERCIAL AND LIGHT-INDUSTRIAL ENVIRONMENTS

---

*EN 50081-1, the generic emission standard for residential, commercial and light industrial states that:*

“The environments encompassed by this standard are residential, commercial and light-industrial locations, both indoor and outdoor. The following list, although not comprehensive, gives an indication of locations, which are included:

- residential properties, e.g. houses, apartments
- retail outlets, e.g. shops, supermarkets
- business premises, e.g. offices, banks

- areas of public entertainment, e.g. cinemas, public bars, dance halls
- outdoor locations, e.g. petrol stations, car parks, amusement and sports centres
- light-industrial locations, e.g. workshops, laboratories, service centres

Locations which are characterized by being supplied directly at low voltage from the public mains network are considered to be residential, commercial or light industrial.”

### INDUSTRIAL ENVIRONMENT

---

*EN 50081-2, the generic emission standard for the industrial environment states that:*

“Apparatus covered by this standard is not intended for connection to the public mains network but is intended to be connected to a power network supplied from a high or medium-voltage transformer dedicated for the supply of an installation feeding manufacturing or similar plant.”

*Industrial locations are characterized by the existence of one or more of the following conditions:*

- industrial, scientific and medical (ISM) apparatus
- heavy inductive or capacitive loads are frequently switched
- currents and associated magnetic fields are high

These are the major contributors to the industrial electromagnetic environment and as such distinguish the industrial from other environments.

*ISM equipment is defined in EN 55011, Annex A as:*

“... suitable for use in all establishments other than domestic and those connected to a low voltage power supply network which supplies buildings used for domestic purposes.”

Some examples from Appendix A of EN 55011 for ISM equipment include: signal generators, measuring receivers, spectrum analyzers, chemical analysis machines and switched mode power supplies.

Examples of general equipment include: industrial induction heating equipment, industrial microwave heating equipment, medical apparatus (specifically short-wave therapy equipment and microwave therapy equipment), spark erosion equipment, and spot welders.

Some overlap exists in the definitions of the two categories and it is up to the manufacturer to use the best judgement in selecting the appropriate category. The manufacturer always has the final responsibility in assuring compliance with the directive.



# Standard Selector Guide

Product Category	Emissions			Immunity
	AC Power harmonic currents	Voltage Flicker	RF Emissions	ESD, EFT, Surge, and RF Immunity
Audio equipment	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55013	EN 50082-1
Household appliances and portable tools, e.g. vacuum cleaners, washing machines, heating and cooking appliances, dimmers	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55014	EN 55104
Industrial electronic power and control equipment	EN 61000-3-2	EN 61000-3-3	EN 50081-2	EN 50082-2
Industrial non-electronic equipment e.g. commutator motors	EN 61000-3-2	EN 61000-3-3	EN 50081-2	EN 50082-2
Industrial, Scientific and Medical (ISM) equipment designed to generate radio frequency energy	EN 61000-3-2	EN 61000-3-3	EN 55011	EN 50082-1 or EN 50082-2
Information Technology Equipment (ITE)	EN 61000-3-2	EN 61000-3-3	EN 55022	EN 50082-1 or EN 50082-2
Lifts	----	----	prEN 12015	prEN 12016
Lighting equipment	EN 60555-2 will become EN 61000-3-2	EN 61000-3-3 for disco lighting etc.	EN 55015	EN 50082-1 will be EN 61547 in the future
Medical Equipment	----	----	EN 60601-1-2	EN 60601-1-2
Power Mains signaling equipment	EN 61000-3-2	----	EN 50065-1	EN 50082-1
Professional Audio Visual Equipment	----	----	prEN 55103-1	prEN 55103-2
Residential and Light Industrial equipment	EN 61000-3-2	EN 61000-3-3	EN 50081-1	EN 50082-1
TV and Radio Receivers	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55013	EN 55020

## PRODUCT AND PRODUCT FAMILY STANDARDS FOR IMMUNITY MAXIMUM REQUIRED TEST LEVELS

IEC	ESD	EFT	Surge Combination Wave	Surge Telecom Wave	Power Frequency Magnetic Field	Pulse Magnetic Field	Dips & Interrupts	100kHz Ring Wave
EN 50082-1: Jan 92 Generic Immunity – Residential, Commercial, and Light Industrial	8kV air discharge	1kV	–	–	–	–	–	–
prEN 50082-1: Oct 96 <sup>1</sup> Generic Immunity – Residential, Commercial, and Light Industrial	4kV contact mode	1kV	2kV common mode	–	3A/m	–	40% and 70% Dips; Interrupts to 0	–
	8kV air discharge		1kV differential mode	–	–	–		
EN 50082-2: 1995 Generic Immunity – Industrial Environment	4kV contact mode	2kV	–	–	30A/m	–	–	–
	8kV air discharge		1kV differential mode	–	–	–		
prEN 50082-2: Aug 96 <sup>1</sup> Generic Immunity – Industrial Environment	4kV contact mode	2kV	4kV common mode	–	30A/m	–	40% and 70% Dips; Interrupts to 0	–
	8kV air discharge		2kV differential mode	–	–	–		
EN 55104 Immunity – Household Appliances, Tools and Similar Apparatus	4kV contact mode	1kV	2kV common mode	–	–	–	40% and 70% Dips; Interrupts to 0	–
	8kV air discharge		1kV differential mode	–	–	–		

<sup>1</sup> Draft



One Lowell Research Center  
 Lowell, Massachusetts 01852-4345 USA  
 1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
 email: sales@keytek.com  
 http://www.keytek.com  
 A division of Thermo Voltek, a Thermo Electron company

KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
 Specifications are subject to change without notice. Printed in USA. 10/97

KPS-662-A-10-97





# KeyTek Application Note

## EMC Standards Overview

### AN OVERVIEW

---

The European Union's EMC Directive requires that virtually all electronic and electrical products be tested for immunity to both man-made and natural phenomena and to insure that products do not emit unintentional signals that may interfere with the continued, reliable operation of other products.

In order to accomplish this objective, CENELEC (an acronym for Comité Européen de Normalisation Electrotechnique) was tasked with identifying the standards to be applied. CENELEC in conjunction with the IEC (International Electrotechnical Commission) and CISPR (Comité International Spécial des

Perturbations Radioélectroniques) have defined a series of Product Standards, Product Family Standards, and Basic EMC Standards for use in complying with the EMC Directive.

Compliance with the EMC Directive will require products be tested in accordance with European Norms, or ENs, issued by CENELEC. These ENs are not developed by CENELEC but are IEC and CISPR standards redesignated as ENs. For example, Basic EMC Standard IEC 1000-4-2 becomes EN 61000-4-2; Basic EMC Standard CISPR 22 becomes EN 55022.

### THE IEC

---

The IEC or International Electrotechnical Commission is a worldwide standards writing organization. Membership includes most industrialized nations and is open to any nation that wishes to contribute and supply a technical expert.

Within the IEC are Technical Committees, each tasked with developing and maintaining specific types of standards. Most Basic EMC Standards for immunity are developed by the IEC, as are most Product and Product Family Standards.

### CISPR

---

CISPR is a special part of the IEC tasked with the development of standards dealing with unwanted radiated emissions in the RF (radio frequency) spectrum. The objective of CISPR standards is to limit the amount of undesirable RF emanating from electrical and

electronic products, and therefore limit the amount of interference to other electronic products. Most Basic EMC Standards for radiated emissions are written by CISPR Technical Committees.

### THE STANDARDS

---

There are three types of EMC Publications:

Product Standards  
Product Family Standards (including Generic Standards)  
Basic EMC Publications



# EMC Standards Overview

## PRODUCT STANDARDS

Product EMC Standards relate to a particular type of product, system or installation for which specific conditions must be considered. Product EMC Standards include:

- Resistance Welding equipment
- Measuring Relays and Protection equipment

Product Standards have priority over Product Family and Generic Standards; however, where no Product Standard or Product Family Standard exists for a particular product, the relevant Generic Standard will apply.

## PRODUCT FAMILY STANDARDS

Product Family Standards apply to products of a particular category such as:

- Household appliances and portable tools
- ITE (Information Technology Equipment)
- Audio, video, audio-visual and entertainment lighting control apparatus for professional use

Product Family Standards have priority over Generic Standards; however, where no Product Family EMC Standard exists for a particular product family, the relevant Generic Standard will apply.

## GENERIC STANDARDS

Generic EMC Standards are a special type of Product Family Standard which apply to products operating in a particular environment for which no dedicated Product or Product Family Standard exists. They specify a set of essential requirements, test procedures and generalized performance criteria applicable to products or systems operating in this environment.

The Generic EMC Standards include: EN 50082-1, EN 50082-2, EN 50081-1 and EN 50081-2 which cover immunity and emissions testing for commercial, residential and light industrial environments, as well as for industrial environments.

## BASIC EMC PUBLICATIONS

Basic EMC Publications may be standards or technical reports which, by definition, are NOT dedicated to specific product families, products, systems or installations. They may concern:

- Terminology
- Descriptions of electromagnetic phenomena
- Specification of compatibility levels (NOT compliance levels)
- General requirements for the limitation of emissions
- Recommendations for test levels for immunity
- Measurement and test techniques
- Descriptions and classification of the environment

Basic EMC Publications include Basic EMC Standards such as the IEC 1000-4-X Series, CISPR 22, CISPR 11, and others. (IEC 1000-4-X Series will become IEC 61000-4-X as new standards are developed and current ones revised.)

## OTHER DIRECTIVES

In addition to the EMC Directive, there are other directives to which manufacturers of electrical and electronic products may have to comply:

Safety Directives: Machinery Directive  
Low Voltage Directive

Each product must comply with the safety directive that is most applicable. Products which can be classified as machinery should comply with the Machinery Directive, and those products that can be classified as electrical or electronic products will have to meet the Low Voltage Directive. The manufacturer is required to determine which is most applicable for each product.

Other directives include:

- Toy Directive (already in force)
- Medical Devices Directive (medical electronics)
- Telecommunications Directive (telecom products)
- Automotive Directive (vehicles and vehicle electronics)

## STANDARD DOCUMENT SOURCES

Standards may be obtained directly from the issuing body - the IEC or CENELEC, or from your national standards organization. In the United States it is the American National Standards Institute (ANSI) at + (1) 212-642-4900; in the United Kingdom it is the British Standards Institute (BSI). Commercial sources include The Document Center in the United States at + (1) 415-591-7600.

In order to maintain an up-to-date Standards file, contact ERA Technology Ltd. in the United Kingdom at +(44) 1372 367018 and request a subscription to the Safety and EMC newsletter.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97



# KeyTek Application Note

## Surge Testing per IEC 1000-4-5

### SURGE BACKGROUND

Surges occur on the AC power mains as a result of switching operations in the power grid and from nearby lightning strikes, either directly to the power distribution system or to nearby ground. Radiated coupling of surges into I/O lines generally occurs only when the lines are very long.

Electronic products are tested for Surge immunity to insure their continued reliable operation if subjected to

realistic levels of surge voltages. The European Union's EMC Directive currently mandates Surge testing for some products; however, it is expected that virtually all electrical and electronic products will have to be tested for Surge immunity in the near future as a condition for obtaining the CE Mark before shipping products to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require Surge tests be performed in accordance with Basic EMC Standards: IEC 801-5, IEC 1000-4-5 or EN 61000-4-5. KeyTek's Application Note, "EMC Standards Overview," provides an overview

of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD

The Basic EMC Standard for Surge defines the methods of generating consistently reproducible surge voltages for test purposes. They specify generator and coupler/decoupler design and performance in sufficient detail to produce correlatable results between test sites.


While the Basic EMC Standard specifies how to perform Surge testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Standard	Applicability	Common Mode	Differential Mode
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	N/A	N/A
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	2kV	1kV
EN 50082-2	Generic Immunity - Industrial Environment	N/A	N/A
EN 50082-2 Draft	Generic Immunity - Industrial Environment	4kV	2kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	2kV	1kV

### SAFETY

When performing Surge tests, safety is a primary concern. Surge voltages and currents must be contained to insure they will not appear where they can cause damage to other instruments in the test area. The test pulses used for Surge testing are of sufficient energy to cause components to fragment under fault conditions and become hazardous to personnel in unprotected environments.

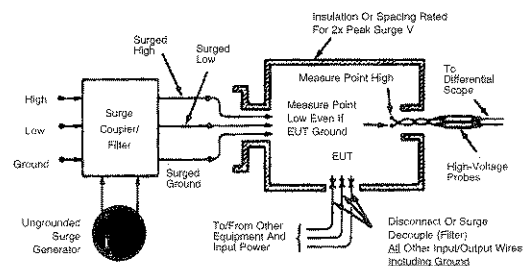


# Surge Testing per IEC 1000-4-5

## COUPLING METHODS

**Capacitive Coupling** via  $9\mu\text{F}$  (Line to earth) or  $18\mu\text{F}$  (line to line) capacitors is required for coupling surges to AC or DC power mains. These coupling capacitors are typically included as part of a Coupler/Decoupler (C/D) in commercially available Surge simulators. The C/D provides both coupling to the EUT power mains and a decoupler to prevent the surge from appearing on the ac mains connected to other equipment in the lab.


**Capacitive Coupling** via  $.5\mu\text{F}$  capacitors, as well as via alternative devices such as surge arrestors, are used to couple surges onto data, I/O and telecommunication lines. Surge arrestors are the preferred coupler device due to the undesirable loading effects of capacitors particularly at frequencies greater than a few kilohertz. A decoupler is included to prevent the surge from appearing at, and potentially damaging, the auxiliary equipment.

## WAVEFORMS

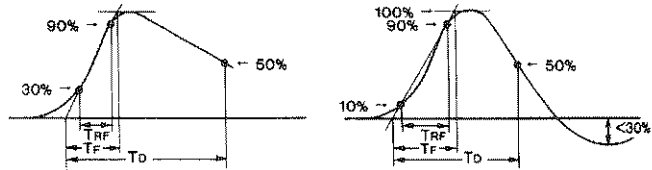

## WAVEFORM VERIFICATION

IEC 1000-4-5 requires that the simulator output be verified periodically. High voltage differential surge probes are required for verifying the open-circuit voltage, and a suitable current transformer (Pearson Model 110 or equivalent) is required for verification of the short-circuit current. A digital or storage oscilloscope with 100MHz bandwidth is sufficient for measuring the surge voltage and current waveforms and peaks.

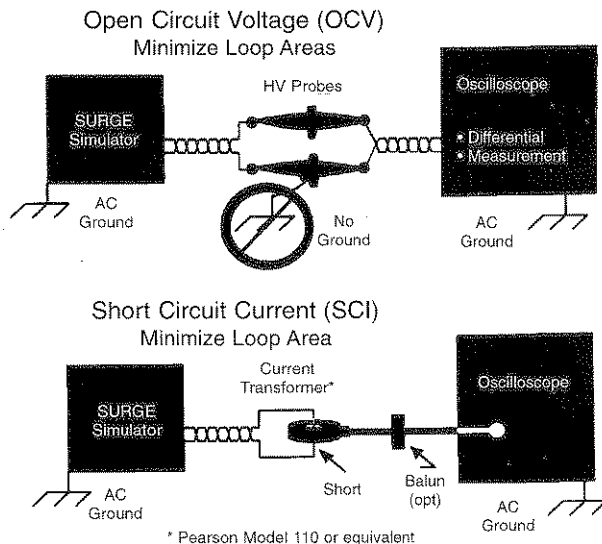

## TEST EXECUTION

According to IEC 1000-4-5, testing must be carried out according to the manufacturer's test plan, which shall specify:

- Generator & other equipment
- Generator Source Impedance
- Repetition rate (one per minute maximum)
- Sequence of application of the surge
- Installation conditions
- Operating conditions of EUT
- Number of tests (at least five positive and five negative at each point)
- Test levels
- Polarity
- Inputs/outputs tested
- Phase angle of coupling to ac mains
- Internal or external trigger

## EUT PERFORMANCE CRITERIA

For Surge tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating status or data storage. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## SURGE SIMULATORS

Surge Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-5, including dynamic source impedance, all waveform characteristics, and coupler/decoupler design. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97

# KeyTek Application Note

## Dips and Interrupts Testing per IEC 1000-4-11

### DIPS AND INTERRUPTS BACKGROUND

---

Dips and interrupts can occur on the AC power mains as a result of a fault in the distribution system such as an open circuit breaker or a sudden large load being turned on in the immediate vicinity. A power distribution system fault can cause a switch in the distribution grid to open and close a number of times, resulting in multiple interrupts to electrical and electronic equipment.

Electronic products are tested for immunity to dips and interrupts to insure their continued reliable operation if subjected to dips and/or interrupts on the AC power mains. The European Union's EMC Directive mandates dips and interrupts testing for virtually all electrical and electronic products as a condition for obtaining the CE Mark before shipping products to member states of the European Union.

### APPLICABLE STANDARDS

---

Generic Immunity Standards, Product Standards and Product Family Standards require that dip and interrupt tests be performed in accordance with Basic EMC Standards: IEC 1000-4-11 and EN 61000-4-11<sup>1</sup>. KeyTek's Application Note, "EMC Standards

<sup>1</sup> IEC 1000-4-11 and EN 61000-4-11 are virtually identical standards.

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD

---

The Basic EMC Standard for Dips and Interrupts defines methods of generating consistently reproducible electrical dips and interrupts for test purposes. They specify characteristics of the AC mains to the EUT such as peak inrush current, transition times and durations.

While the Basic EMC Standard specifies how to perform Dips and Interrupts testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail Performance Criteria.

### TEST LEVELS

---

Standard	Applicability	Levels
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	Not required
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	0%, 40%, 70% & 100%
EN 50082-2	Generic Immunity - Industrial Environment	Not required
EN 50082-2 Draft	Generic Immunity - Industrial Environment	0%, 40%, 70% & 100%
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	0%, 40%, 70% & 100%

# Dips and Interrupts Testing per IEC 1000-4-11


## PEAK INRUSH CURRENT

IEC 1000-4-11 requires the simulator be capable of supplying peak inrush currents of up to 500A for 220V to 240V mains, and up to 250A for 100V to 120V mains. Additionally, the Standard requires this capability be measured using a bridge rectifier connected via a switch to a discharged 1700 $\mu$ F capacitor. The parallel discharge resistance should be chosen to allow several RC time constants between tests. An example in Annex A (normative) uses a 10k ohm resistance, providing a time constant of 17 s, "...so that a wait of 1.5 to 2 minutes should be used between inrush drive capability tests."

The test for inrush current is performed by switching the generator from 0% to 100% at both 90° and 270° to insure sufficient peak inrush current drive capability for both polarities.

## WAVEFORM VERIFICATION

IEC 1000-4-11 requires that the simulator output be verified periodically. For Dip and Interrupt test simulators, it is necessary to verify the voltage transition levels, transition times to 100%, and the inrush current capability. Most modern oscilloscopes are capable of observing the voltage levels and transition times. For verifying the inrush current, a bridge rectifier, suitably rated 1700 $\mu$ F capacitor and appropriate current transformer are required.

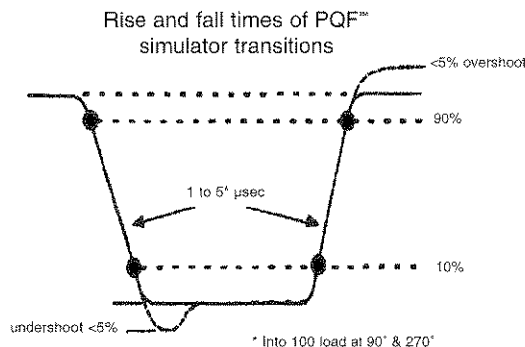

## TEST EXECUTION

According to IEC 1000-4-11, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- Input power of the EUT
- Performance Criteria
- Operation modes of the EUT
- Test set-up description
- Type of designation of the EUT
- Information on possible connections, cables, peripherals, etc.

After each group of tests, a complete functional test must be performed.

## EUT PERFORMANCE CRITERIA

For Dip and Interrupt tests, Performance Criteria varies in some standards depending on the duration or severity of the dip and/or interrupt. Under some conditions, loss of function is allowed, provided that the function is self-recoverable or can be restored by the control operations. Under less severe conditions, degradation of performance is allowed during the test, however, the unit must continue to operate as intended after the test. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## DIP AND INTERRUPT SIMULATORS

Dip and Interrupt Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-11, including those for peak inrush current. Additionally, KeyTek simulators meet the fast switching time requirements not only to 100% as required by the standards, but from any level to any other level. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark and PQF is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice.  
Printed in USA. 10/97



# KeyTek Application Note

## ESD Testing per IEC 1000-4-2

### ESD BACKGROUND

Electrostatic Discharge (ESD) is the abrupt release of charge from one object (often a person) to another. Such a discharge can permanently damage or otherwise upset the function of sensitive electronic circuits.

Electronic products are tested for ESD immunity to insure their continued reliable operation if subjected to

realistic levels of ESD after being placed in service. The European Union's EMC Directive mandates ESD immunity testing for virtually all electrical and/or electronic products as a condition for obtaining the CE Mark before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity Standards, Product Standards and Product Family Standards require that ESD tests be performed in accordance with specific Basic EMC Standards: IEC 801-2, IEC 1000-4-2, or EN 61000-4-2. KeyTek's Application Note, "EMC Standards

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD



The Basic EMC Standards for ESD define methods of generating consistently reproducible electrical stresses for test purposes. They specify capacitances and resistances to model the human body's charge storing capability and discharge impedance, respectively.

This model results in a current waveform, defined in the Standards. While the Basic EMC Standard also specifies how to perform ESD testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail Performance Criteria.

### TEST LEVELS

Standard	Applicability	Contact Discharge Test Voltage	Air Discharge Test Voltage
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	N/A	8kV
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	4kV	8kV
EN 50082-2	Generic Immunity - Industrial Environment	4kV	8kV
EN 50082-2 Draft	Generic Immunity - Industrial Environment	4kV	8kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	4kV	8kV

### TEST SET-UP

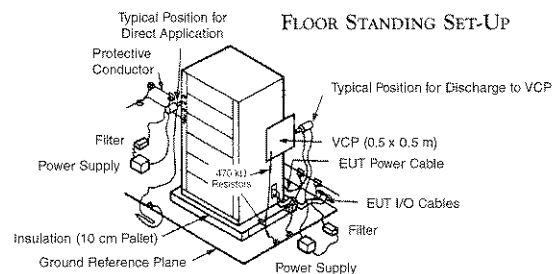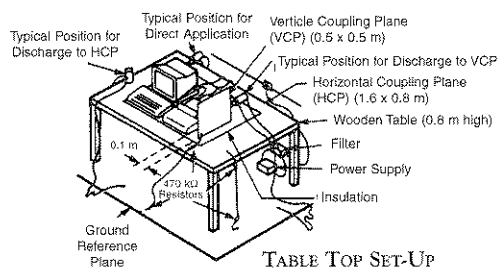


# ESD Testing per IEC 1000-4-2

## COUPLING METHODS

Direct Coupling is a discharge directly to the Equipment Under Test (EUT), either in an Air Discharge mode, necessary for products having few or no metal surfaces, or via Contact mode, the preferred method. In the "air discharge" mode, the ESD event is initiated when the test simulator output is brought into close proximity with the EUT until a spark is initiated. The resulting stress is influenced by various environmental factors. In the preferred "contact discharge" mode, the test simulator output is first brought into physical contact with the EUT, then the ESD event is initiated under controlled conditions within the simulator.

Indirect Coupling simulates an ESD event which causes a radiated field to be emitted in the vicinity of the victim equipment. This is accomplished using Vertical Coupling Planes (VCP's) and Horizontal Coupling Planes (HCP's). Current standards require discharges be made to the edge of the VCP and surface of an HCP.

## WAVEFORMS

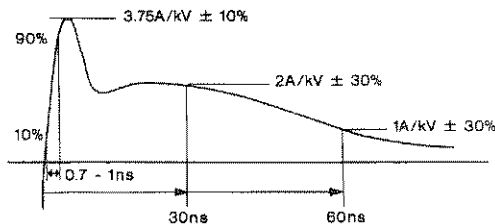

## WAVEFORM VERIFICATION

IEC 1000-4-2 requires the simulator output be verified periodically. A Model CTC-3 measurement target and target plane is required. The ESD current measurement is then made using a measurement system having a 1GHz or greater bandwidth. It is necessary to place the oscilloscope inside a shielded enclosure during the measurement to reduce the effects of radiated ESD directly to the measurement instrument.

Recent work by the Working Group 14.0 of the ESD Association has found that some simulators produce waveforms that are in compliance with IEC 1000-4-2, but have considerable ringing and high frequency components that do not show up with 1GHz instrumentation. These simulators may cause failures in products which would not occur if tested with a KeyTek simulator. Working Group 14.0 is preparing a document to describe waveform verification methods to allow manufacturers to verify the ESD current from simulators using high bandwidth instrumentation.

## NUMBER AND RATE OF DISCHARGES

The manufacturer is required to develop a test plan identifying the EUT's most sensitive operating mode and appropriate test points. A minimum of 10 discharges are then made to each test point in either Contact Discharge or Air Discharge, according to the test plan. A recommended time interval of 1 second between tests should be used, but a longer interval is allowed if necessary to determine if a system failure has occurred.

For the indirect tests, 10 discharges are required to the Vertical Coupling Plane at each of 4 equipment faces (40 discharges) and then 10 discharges are required to the Horizontal Coupling Plane at 4 sides of the EUT (40 discharges).

## EUT PERFORMANCE CRITERIA

For ESD tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating state or stored data. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## ESD SIMULATORS

ESD Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-2, including discharge network characteristics, discharge tips, and waveforms. Numerous accessories and discharge tips are available from KeyTek for those manufacturers requiring additional test capability and flexibility. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97

# KeyTek Application Note

## ESD Accessories for Testing Beyond IEC 1000-4-2

### REAL WORLD TESTING

ESD is the most common cause of failure in computer based equipment. It accounts for hundreds of millions of dollars in downtime and repair costs each year.

Fortunately, catastrophic failures are preventable and many manufacturers have R&D and manufacturing programs to insure that their products are ESD resistant when shipped. The European Union's EMC Directive requires that virtually all electronic and electrical products be tested for a minimum level of ESD immunity.

However, experience by manufacturers has shown that the characteristics of real ESD vary somewhat from the test pulses required by mandatory standards. Current rise times are much faster and fields associated with discharges are more significant than thought.

In order to insure that products are immune to real ESD events, it is necessary to test beyond the requirements of the mandatory standards using different discharge tips, coupling planes and other accessories.

### APPLICABLE STANDARDS

Generic Immunity Standards, Product Standards and Product Family Standards require that ESD tests be performed in accordance with specific Basic Test Standards: IEC 801-2, IEC 1000-4-2 or EN 61000-4-2.

KeyTek's Application Note "EMC Standards Overview" provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARDS

The Basic EMC Standards for ESD define methods of generating consistently reproducible electrical stresses

for test purposes. (Refer to ESD Testing per IEC 1000-4-2 Application Note.)

### APPLYING DISCHARGES

ESD is applied both directly to the Equipment Under Test (EUT) and indirectly, via horizontal and vertical coupling planes.



Direct coupling is performed with either a contact mode discharge to metal surfaces of the EUT (preferred method), or via an air discharge. In both cases, discharges must be made to all points and surfaces accessible to personnel during normal usage. Tests are performed using 10 single discharges per test point in the most sensitive polarity.

Indirect discharges are performed to simulate radiated ESD events to the EUT. Using the vertical coupling

plane (VCP), at least 10 discharges to the center of the edge of the plane are required with the VCP positioned to completely radiate towards four faces of the EUT.

The horizontal coupling plane (HCP) is on the surface of the work table and is covered with a material to electrically insulate it from the EUT. Currently, a discharge is made to the surface of the HCP at a distance of 0.1m from each side of the EUT, however, an amendment is in process to modify this procedure and require discharges to be made to the center of the edge of the HCP.

### TEST SET-UP

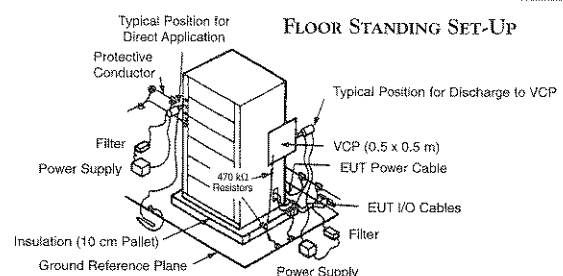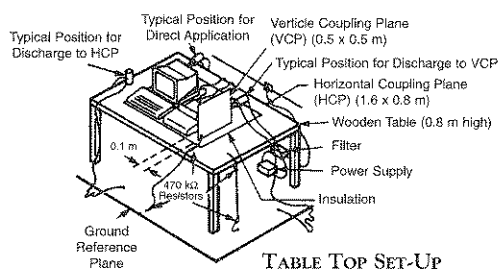

# ESD Accessories for Testing Beyond IEC 1000-4-2

## CM-ESD AND PRO-ESD TIPS

---

Simulator tips are included with CM-ESD and PRO-ESD for both contact mode testing (TPC-3) and air discharge testing (TPA-2) in accordance with IEC 1000-4-2. For very fast, real-world rise times, the TPA-1 for air discharge will provide rise times on the order of 0.4ns or faster.

A method used successfully for locating ESD and RF susceptibility problems is self-discharge: producing the spark associated with an air discharge, but without actually discharging to the equipment under test. This is done using the TPF-1 self-discharge tip in the vicinity of suspect cables, connectors, shields and the like.

Another useful tool is the 50-MZ standoff spacer for air-discharge testing. This allows the user to set the precise distance between the tip and the target equipment, useful for investigative work.

When trying to determine the real cause of an ESD immunity problem, it is useful to separate E-Field and H-Field effects. This is easily accomplished with the MZT-11 E-Field and MZT-12 H-Field Simulator Tip Assemblies.

In order to determine if fields are being generated and to observe the relative levels of those fields, the FCS-1 Field and Corona Sensor Group was developed.

This option includes a basic monitor unit, HEC-1, H-Field Sensor, HFS-1, E-Field Sensor, EFS-1, and Pre-discharge Corona Sensor, CCS-1.

## COUPLING PLANES

---

Two coupling planes, one horizontal and one vertical, are required for product testing in accordance with IEC 1000-4-2. The Horizontal Coupling Plane, a model HCP-1, is placed on a non-conductive table below the equipment being tested. A discharge to the HCP-1 will then cause a horizontally polarized field to be radiated up into the product being tested. A Vertical Coupling Plane, model VCP-1, is oriented at a fixed distance from the product being tested. A discharge is made to the edge of the VCP-1 causing a vertically polarized field to be radiated towards the product. All four sides of the product must be tested in this manner.

Another type of plane available as an accessory to the CM-ESD and PRO-ESD is the TP-3, a 1.5m x 1.5m Target Plane used with the CTC-3 ESD target for waveform verification. The CTC-3 is mounted in the center of the plane and the ESD current is monitored on an oscilloscope which is installed inside a Faraday cage.

## OTHER ACCESSORIES

---

In order to obtain an independent measurement of the ESD voltage on the tip of the CM-ESD and PRO-ESD, a calibrated attenuator, such as the DCA-2 is required. With the attenuator in place, the output voltage can be read using any DC attenuator.

For customers planning to ship the CM-ESD and PRO-ESD between facilities on a regular basis, the MCA-1 Hard Carrying Case is recommended. No additional shipping materials are required. Secure the unit in the MCA-1, affix the proper labels, and call the shipper.

Some corporate standards require testing with hundreds or even thousands of discharges to a point on the equipment under test. A non-conducting tripod, such as the T-2, allows the CM-ESD and PRO-ESD simulator to be held steady against the equipment being tested, without interfering with the test results.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
<http://www.keytek.com>

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 4/98

# KeyTek Application Note

## EFT Testing per IEC 1000-4-4

### EFT BACKGROUND

Electrical Fast Transients (EFT) are caused anytime a gaseous discharge occurs (a spark in air or other gas), the most common being the opening of a switch through which current is flowing. As the switch is opened, arcing occurs between the contacts; first at a low voltage and high frequency while contacts are close together, and later at a higher voltage and lower frequency as the contacts become separated. Coupling of the EFT into electronic products occurs when power cables handling

high currents are run in close proximity to power, data, and/or I/O cables.

Electronic products are tested for EFT immunity to insure their continued reliable operation if subjected to realistic levels of fast transients. The European Union's EMC Directive mandates EFT testing for virtually all electrical and electronic products as a condition for obtaining the CE Mark before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require that EFT tests be performed in accordance with Basic EMC Standards: IEC 801-4, IEC 1000-4-4 or EN 61000-4-4<sup>1</sup>. KeyTek's Application Note,

<sup>1</sup> IEC 801-4, IEC 1000-4-4, and EN 61000-4-4 are essentially the same for test voltages and levels.

"EMC Standards Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

### BASIC EMC STANDARD



The Basic EMC Standards for EFT define methods of generating consistently reproducible fast transients for test purposes. They specify generator and coupler/decoupler design and performance in an attempt to produce correlational results between test sites. The

Basic EMC Standard specifies how to perform EFT testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Standard	Applicability	Test Voltage
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	1kV
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	1kV
EN 50082-2	Generic Immunity - Industrial Environment	2kV
EN 50082-2 Draft	Generic Immunity - Industrial Environment	2kV
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	1kV

### TEST SET-UP

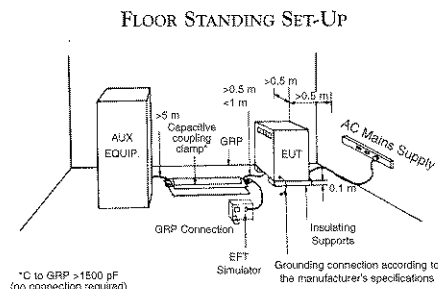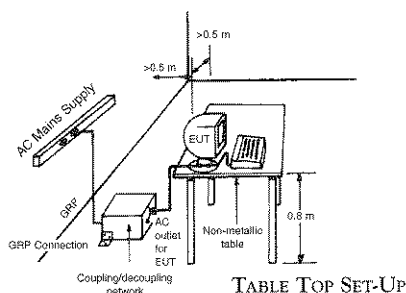

\*C to GRP >1500 pF (no connection required)  
Grounding connection according to the manufacturer's specifications

# EFT Testing per IEC 1000-4-4


## COUPLING METHODS

**Capacitive Coupling** via 33nF capacitors is the required coupling method to AC or DC power mains. These coupling capacitors are included as part of a Coupler/ Decoupler (C/D) in commercially available EFT simulators. The design of the decoupling portion of the C/D, which prevents the EFT burst from traveling back onto the power mains, is also specified in IEC 1000-4-4.

A **Capacitive Coupling Clamp** is used to couple EFT bursts onto data, I/O, and telecommunications lines. Construction of the clamp is shown in Figure 5 of IEC 1000-4-4; however, considerable differences exist in commercially available clamps. Some clamps use higher quality materials and some designs allow for the use of an optional safety interlocked cover.

## WAVEFORMS

### STANDARD EFT WAVEFORM

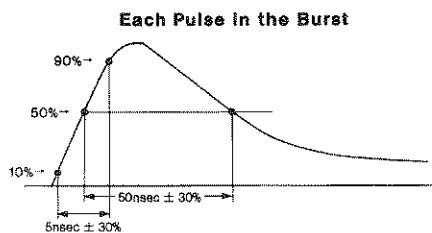

## WAVEFORM VERIFICATION

IEC 1000-4-4 requires that the simulator output be verified periodically. A 50 ohm load and attenuator rated for high voltage is required and the measurement must be made using an oscilloscope with at least 400MHz bandwidth.

One problem noted with IEC 1000-4-4 is that simulator designs can be quite different and although each has a 50 ohm source impedance and provides the specified pulse into a 50 ohm termination, some simulators provide significantly more or less energy than others into loads that are not 50 ohms - the AC power input of most electronic products is something other than 50 ohms. To deal with the problems, changes to the standard were proposed to require waveforms be verified into a 1000 ohm load. Unfortunately, these changes were not accepted; however, this and other proposed improvements to IEC 1000-4-4 will be included in a forthcoming Annex.

## TEST EXECUTION

According to IEC 1000-4-4, testing must be carried out according to the manufacturer's test plan, which shall specify:

<b>Type of test</b>	Test levels
<b>Polarity (+ &amp; - required)</b>	Test duration (1 minute minimum)
<b>Number of Voltage tests</b>	EUT ports
<b>EUT operating condition</b>	Sequence to tests to ports, etc.
<b>Auxiliary equipment</b>	

## EUT PERFORMANCE CRITERIA

For EFT tests, the Generic Immunity Standards and Household Appliances Product Family Standard require that products operate as intended after the test. No degradation or loss of function is allowed below a performance level specified by the manufacturer. During the test, degradation is allowed, but not a change in the actual operating status or data storage. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## EFT SIMULATORS

EFT Simulators produced by KeyTek Instrument Corporation meet all the simulator requirements of IEC 1000-4-4, including discharge pulse energy, output type, dynamic source impedance, and all waveform characteristics. Additionally, KeyTek simulators meet the requirements for coupling/decoupling networks for AC and DC mains as described in paragraph 6.2 of IEC 1000-4-4. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA. 10/97

# KeyTek Application Note

## EMC Standards Overview

### AN OVERVIEW

---

The European Union's EMC Directive requires that virtually all electronic and electrical products be tested for immunity to both man-made and natural phenomena and to insure that products do not emit unintentional signals that may interfere with the continued, reliable operation of other products.

In order to accomplish this objective, CENELEC (an acronym for Comité Européen de Normalisation Electrotechnique) was tasked with identifying the standards to be applied. CENELEC in conjunction with the IEC (International Electrotechnical Commission) and CISPR (Comité International Spécial des

Perturbations Radioélectroniques) have defined a series of Product Standards, Product Family Standards, and Basic EMC Standards for use in complying with the EMC Directive.

Compliance with the EMC Directive will require products be tested in accordance with European Norms, or ENs, issued by CENELEC. These ENs are not developed by CENELEC but are IEC and CISPR standards redesignated as ENs. For example, Basic EMC Standard IEC 1000-4-2 becomes EN 61000-4-2; Basic EMC Standard CISPR 22 becomes EN 55022.

### THE IEC

---

The IEC or International Electrotechnical Commission is a worldwide standards writing organization. Membership includes most industrialized nations and is open to any nation that wishes to contribute and supply a technical expert.

Within the IEC are Technical Committees, each tasked with developing and maintaining specific types of standards. Most Basic EMC Standards for immunity are developed by the IEC, as are most Product and Product Family Standards.

### CISPR

---

CISPR is a special part of the IEC tasked with the development of standards dealing with unwanted radiated emissions in the RF (radio frequency) spectrum. The objective of CISPR standards is to limit the amount of undesirable RF emanating from electrical and

electronic products, and therefore limit the amount of interference to other electronic products. Most Basic EMC Standards for radiated emissions are written by CISPR Technical Committees.

### THE STANDARDS

---

There are three types of EMC Publications:

Product Standards  
Product Family Standards (including Generic Standards)  
Basic EMC Publications

# EMC Standards Overview

## PRODUCT STANDARDS

---

Product EMC Standards relate to a particular type of product, system or installation for which specific conditions must be considered. Product EMC Standards include:

- Resistance Welding equipment
- Measuring Relays and Protection equipment

Product Standards have priority over Product Family and Generic Standards; however, where no Product Standard or Product Family Standard exists for a particular product, the relevant Generic Standard will apply.

## PRODUCT FAMILY STANDARDS

---

Product Family Standards apply to products of a particular category such as:

- Household appliances and portable tools
- ITE (Information Technology Equipment)
- Audio, video, audio-visual and entertainment lighting control apparatus for professional use

Product Family Standards have priority over Generic Standards; however, where no Product Family EMC Standard exists for a particular product family, the relevant Generic Standard will apply.

## GENERIC STANDARDS

---

Generic EMC Standards are a special type of Product Family Standard which apply to products operating in a particular environment for which no dedicated Product or Product Family Standard exists. They specify a set of essential requirements, test procedures and generalized performance criteria applicable to products or systems operating in this environment.

The Generic EMC Standards include: EN 50082-1, EN 50082-2, EN 50081-1 and EN 50081-2 which cover immunity and emissions testing for commercial, residential and light industrial environments, as well as for industrial environments.

## BASIC EMC PUBLICATIONS

---

Basic EMC Publications may be standards or technical reports which, by definition, are NOT dedicated to specific product families, products, systems or installations. They may concern:

- Terminology
- Descriptions of electromagnetic phenomena
- Specification of compatibility levels (NOT compliance levels)
- General requirements for the limitation of emissions
- Recommendations for test levels for immunity
- Measurement and test techniques
- Descriptions and classification of the environment

Basic EMC Publications include Basic EMC Standards such as the IEC 1000-4-X Series, CISPR 22, CISPR 11, and others. (IEC 1000-4-X Series will become IEC 61000-4-X as new standards are developed and current ones revised.)

## OTHER DIRECTIVES

---

In addition to the EMC Directive, there are other directives to which manufacturers of electrical and electronic products may have to comply:

Safety Directives:            Machinery Directive  
   Low Voltage Directive

Each product must comply with the safety directive that is most applicable. Products which can be classified as machinery should comply with the Machinery Directive, and those products that can be classified as electrical or electronic products will have to meet the Low Voltage Directive. The manufacturer is required to determine which is most applicable for each product.

Other directives include:

- Toy Directive (already in force)
- Medical Devices Directive (medical electronics)
- Telecommunications Directive (telecom products)
- Automotive Directive (vehicles and vehicle electronics)

## STANDARD DOCUMENT SOURCES

---

Standards may be obtained directly from the issuing body - the IEC or CENELEC, or from your national standards organization. In the United States it is the American National Standards Institute (ANSI) at + (1) 212-642-4900; in the United Kingdom it is the British Standards Institute (BSI). Commercial sources include The Document Center in the United States at + (1) 415-591-7600.

In order to maintain an up-to-date Standards file, contact ERA Technology Ltd. in the United Kingdom at +(44) 1372 367018 and request a subscription to the Safety and EMC newsletter.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97



# KeyTek Application Note

## Standard Selector Guide

### PRODUCT AND PRODUCT FAMILY STANDARDS

---

As of January 1, 1996, all electrical or electronics products shipped into the European Union that could either cause electromagnetic interference (EMI) or could be susceptible to EMI, must be tested to ensure adherence to the EMC Directive. (If a manufacturer believes that a product does not cause EMI and is not affected by EMI, the onus is on the manufacturer to substantiate his claims.)

In order to comply with the EMC Directive, the following products listed must conform to applicable Product or Product Family Standards. If no Product or

Product Family Standards exist, the product must comply with the Generic Immunity and Emissions standards. These generic standards are divided into two areas:

<b>Environment</b>	<b>Generic Emissions</b>	<b>Generic Immunity</b>
Residential, commercial, and light industrial	EN 50081-1	EN 50082-1
Industrial	EN 50081-2	EN 50082-2

### RESIDENTIAL, COMMERCIAL AND LIGHT-INDUSTRIAL ENVIRONMENTS

---

*EN 50081-1, the generic emission standard for residential, commercial and light industrial states that:*

“The environments encompassed by this standard are residential, commercial and light-industrial locations, both indoor and outdoor. The following list, although not comprehensive, gives an indication of locations, which are included:

- residential properties, e.g. houses, apartments
- retail outlets, e.g. shops, supermarkets
- business premises, e.g. offices, banks

- areas of public entertainment, e.g. cinemas, public bars, dance halls
- outdoor locations, e.g. petrol stations, car parks, amusement and sports centres
- light-industrial locations, e.g. workshops, laboratories, service centres

Locations which are characterized by being supplied directly at low voltage from the public mains network are considered to be residential, commercial or light industrial.”

### INDUSTRIAL ENVIRONMENT

---

*EN 50081-2, the generic emission standard for the industrial environment states that:*

“Apparatus covered by this standard is not intended for connection to the public mains network but is intended to be connected to a power network supplied from a high or medium-voltage transformer dedicated for the supply of an installation feeding manufacturing or similar plant.”

*Industrial locations are characterized by the existence of one or more of the following conditions:*

- industrial, scientific and medical (ISM) apparatus
- heavy inductive or capacitive loads are frequently switched
- currents and associated magnetic fields are high

These are the major contributors to the industrial electromagnetic environment and as such distinguish the industrial from other environments.

*ISM equipment is defined in EN 55011, Annex A as:*

“... suitable for use in all establishments other than domestic and those connected to a low voltage power supply network which supplies buildings used for domestic purposes.”

Some examples from Appendix A of EN 55011 for ISM equipment include: signal generators, measuring receivers, spectrum analyzers, chemical analysis machines and switched mode power supplies.

Examples of general equipment include: industrial induction heating equipment, industrial microwave heating equipment, medical apparatus (specifically short-wave therapy equipment and microwave therapy equipment), spark erosion equipment, and spot welders.

Some overlap exists in the definitions of the two categories and it is up to the manufacturer to use the best judgement in selecting the appropriate category. The manufacturer always has the final responsibility in assuring compliance with the directive.

# Standard Selector Guide

Product Category	Emissions			Immunity
	AC Power harmonic currents	Voltage Flicker	RF Emissions	ESD, EFT, Surge, and RF Immunity
Audio equipment	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55013	EN 50082-1
Household appliances and portable tools, e.g. vacuum cleaners, washing machines, heating and cooking appliances, dimmers	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55014	EN 55104
Industrial electronic power and control equipment	EN 61000-3-2	EN 61000-3-3	EN 50081-2	EN 50082-2
Industrial non-electronic equipment e.g. commutator motors	EN 61000-3-2	EN 61000-3-3	EN 50081-2	EN 50082-2
Industrial, Scientific and Medical (ISM) equipment designed to generate radio frequency energy	EN 61000-3-2	EN 61000-3-3	EN 55011	EN 50082-1 or EN 50082-2
Information Technology Equipment (ITE)	EN 61000-3-2	EN 61000-3-3	EN 55022	EN 50082-1 or EN 50082-2
Lifts	----	----	prEN 12015	prEN 12016
Lighting equipment	EN 60555-2 will become EN 61000-3-2	EN 61000-3-3 for disco lighting etc.	EN 55015	EN 50082-1 will be EN 61547 in the future
Medical Equipment	----	----	EN 60601-1-2	EN 60601-1-2
Power Mains signaling equipment	EN 61000-3-2	----	EN 50065-1	EN 50082-1
Professional Audio Visual Equipment	----	----	prEN 55103-1	prEN 55103-2
Residential and Light Industrial equipment	EN 61000-3-2	EN 61000-3-3	EN 50081-1	EN 50082-1
TV and Radio Receivers	EN 60555-2 will become EN 61000-3-2	EN 60555-3 will become EN 610003-3	EN 55013	EN 55020

## PRODUCT AND PRODUCT FAMILY STANDARDS FOR IMMUNITY MAXIMUM REQUIRED TEST LEVELS

IEC	ESD	EFT	Surge Combination Wave	Surge Telecom Wave	Power Frequency Magnetic Field	Pulse Magnetic Field	Dips & Interrupts	100kHz Ring Wave
EN 50082-1: Jan 92 Generic Immunity – Residential, Commercial, and Light Industrial	8kV air discharge	1kV	–	–	–	–	–	–
prEN 50082-1: Oct 96 <sup>1</sup> Generic Immunity – Residential, Commercial, and Light Industrial	4kV contact mode 8kV air discharge	1kV	2kV common mode 1kV differential mode	– –	3A/m –	– –	40% and 70% Dips; Interrupts to 0	–
EN 50082-2: 1995 Generic Immunity – Industrial Environment	4kV contact mode 8kV air discharge	2kV	– 1kV differential mode	– –	30A/m –	– –	–	–
prEN 50082-2: Aug 96 <sup>1</sup> Generic Immunity – Industrial Environment	4kV contact mode 8kV air discharge	2kV	4kV common mode 2kV differential mode	– –	30A/m –	– –	40% and 70% Dips; Interrupts to 0	–
EN 55104 Immunity – Household Appliances, Tools and Similar Apparatus	4kV contact mode 8kV air discharge	1kV	2kV common mode 1kV differential mode	– –	– –	– –	40% and 70% Dips; Interrupts to 0	–

<sup>1</sup> Draft



One Lowell Research Center  
 Lowell, Massachusetts 01852-4345 USA  
 1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
 email: sales@keytek.com  
 http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
 KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
 Specifications are subject to change without notice. Printed in USA. 10/97

# KeyTek Application Note

## Power Frequency Magnetic Field Testing per IEC 1000-4-8

### POWER FREQUENCY MAGNETIC FIELD BACKGROUND

Electronic products are often subjected to magnetic fields at AC mains frequencies. These fields are frequently produced in the vicinity of power transformers and can cause problems with video displays, Hall effect sensors, and other electronic products having a sensitivity to magnetic fields. Electronic Products are tested for immunity to power

frequency magnetic fields to insure their continued reliable operation when placed in service. The European Union's EMC Directive currently mandates power frequency magnetic field testing for certain categories of equipment as a condition for obtaining the CE Mark before shipping products to member states of the European Union.

### APPLICABLE STANDARDS

Generic Immunity, Product and Product Family Standards require that Power Frequency Magnetic Field tests be performed in accordance with Basic EMC Standards: IEC 1000-4-8 and EN 61000-4-8<sup>1</sup>. KeyTek's Application Note, "EMC Standards

Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and list sources for procuring copyrighted documents.

### BASIC EMC STANDARD

The Basic EMC Standard for Power Frequency Magnetic Field defines methods of generating consistently reproducible magnetic fields for test purposes. Although higher magnetic field levels are described, compliance to the Generic Immunity Standard for residential and commercial products is 1A/m or 3A/m. Currently applicable only to apparatus

containing devices susceptible to magnetic fields, testing of other products may be required to make that determination. While the Basic EMC Standard specifies how to perform Power Frequency Magnetic Field testing, the Generic, Product and Product Family Standards specify the test levels and pass/fail performance criteria.

### TEST LEVELS

Power Frequency Magnetic Field testing is required for products that could be affected by magnetic fields, including CRTs and Hall Effect Sensors and is strongly recommended for all products.

Standard	Applicability	Magnetic Field Level
EN 50082-1	Generic Immunity - Residential, Commercial and Light Industrial	Not required
EN 50082-1 Draft	Generic Immunity - Residential, Commercial and Light Industrial	3A/m
EN 50082-2	Generic Immunity - Industrial Environment	30A/m
EN 50082-2 Draft	Generic Immunity - Industrial Environment	30A/m
EN 55104	Immunity for Household Appliances, Tools and Similar Apparatus	Not required

### TEST SET-UP


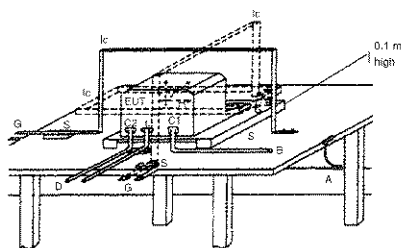


TABLE TOP SET-UP

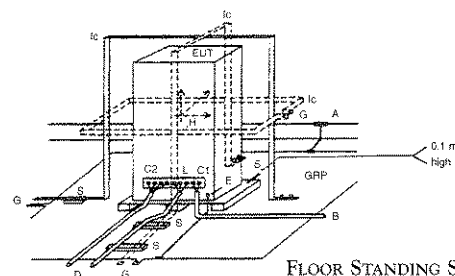

FLOOR STANDING SET-UP

# Power Frequency Magnetic Field Testing per IEC 1000-4-8

## COUPLING METHODS


An Induction Coil having standard dimensions of 1 meter per side for a rectangular coil, or 1 meter diameter for a circular coil, is to be used for testing small equipment. For large equipment, larger dimensions may be used; however, the coil shall be able to envelop the EUT and the coil dimensions must give a minimum distance of coil conductors to EUT walls equal to 1/3 of the dimension of the EUT being tested.

## WAVEFORMS



## WAVEFORM VERIFICATION

IEC 1000-4-8 requires that the simulator output and magnetic field be verified periodically. Any oscilloscope is capable of verifying the power frequency AC current to the coil. Monitoring the actual field requires an AC field probe and monitor, such as the CM-HMON available from KeyTek.

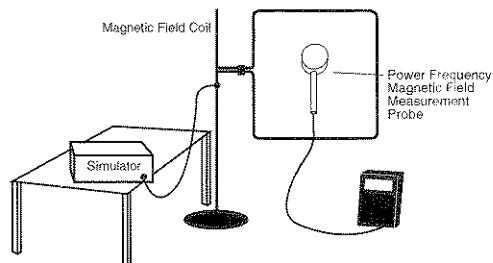

## TEST EXECUTION

According to IEC 1000-4-8, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- How the test is carried out
- Verification of the laboratory reference conditions
- Preliminary verification of the correct operation of the EUT
- An evaluation of the test results

## EUT PERFORMANCE CRITERIA

For Power Frequency Magnetic Field tests, the Generic Immunity Standards require that the product continue to operate as intended during the test, however, CRT interference is allowed above 1A/m in the residential, commercial and light industrial draft standard, and above 3A/m in the industrial standard. No degradation or loss of function is allowed below a performance level specified by the manufacturer. The performance level may be replaced by a permissible loss of performance. Refer to the tables located in the Generic, Product and Product Family Standards for specific Performance Criteria. The product cannot become unsafe under any conditions.

## POWER FREQUENCY MAGNETIC FIELD SIMULATORS

Power Frequency Magnetic Field Simulators and standard coils provided by KeyTek Instrument Corporation meet all the minimum requirements for performing tests to >3A/m in compliance with the applicable Generic and Product Family Standards.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97

# KeyTek Application Note

## Pulse Magnetic field Testing per IEC 1000-4-9

### PULSE MAGNETIC FIELD BACKGROUND

Pulse Magnetic Fields are produced as a result of a large current impulse through a conductor. An example is lightning current flowing through a grounding conductor at a power sub-station. Pulse magnetic fields can also occur in heavy industrial areas where very large current impulses are used in a manufacturing process.

Electronic products are tested for immunity pulse magnetic fields to insure their continued reliable

operation when placed in service in a very harsh environment. Although most electrical and electronic products will not have to be tested for pulse magnetic field immunity, the European Union's EMC Directive may mandate this testing as a condition for obtaining the CE Mark under special circumstances and for specific products before shipping to a member state of the European Union.

### APPLICABLE STANDARDS

Although not currently required by Generic Immunity, Product specific, or Product Family Standards, future standards may require Pulse Magnetic Field tests be performed in accordance with Basic EMC Standards: IEC 1000-4-9 and EN 61000-4-9<sup>1</sup>. KeyTek's Application

Note, "EMC Standards Overview," provides an overview of European Standards for electromagnetic compatibility, describes how the Standards relate to one another, and lists sources for procuring copyrighted documents.

<sup>1</sup> IEC 1000-4-9 and EN 61000-4-9 are virtually identical standards.

### BASIC EMC STANDARD

The Basic EMC Standard for Pulse Magnetic Field defines methods of generating consistently reproducible current impulses for test purposes. Field amplitudes required by these standards range from

100 - 1000 Amps per meter. Although applicable only to apparatus containing devices susceptible to magnetic fields, testing may be required to make that determination.

### TEST LEVELS

Installation Environment	IEC 1000-4-9 Level	Field Strength A/m
Environment where sensitive devices using electron beams can be used	1	N/A
Residential, office and hospital areas far away from earth conductors of lightning protection systems	2	N/A
Commercial areas, control building, field of industrial plants with lightning protection system or metallic structures nearby	3	100
Heavy industrial and power plants and H.V. substation control rooms	4	300
Switchyard areas of heavy industrial plants	5	1000
Higher or lower environmental levels than those described above	X	X

### TEST SET-UP


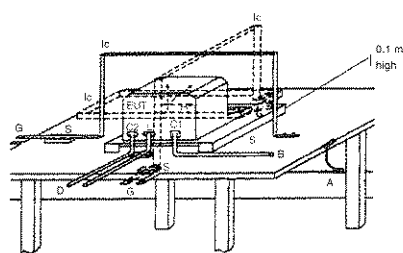


TABLE TOP SET-UP

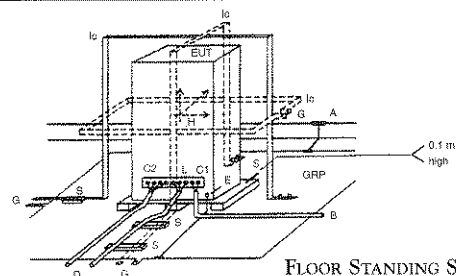

FLOOR STANDING SET-UP


# Pulse Magnetic Field Testing per IEC 1000-4-9

## COUPLING METHODS

An Induction Coil having a standard dimension of 1 meter per side for a rectangular coil, or 1 meter diameter for a circular coil, is to be used for testing small equipment. This coil has a test volume of 0.6m x 0.6m x 0.5m (h). For floor standing equipment, larger dimensions can be used; however, the coil shall be able to envelop the EUT and the coil dimensions must give a minimum distance of coil conductors to EUT walls equal to 1/3 of the dimension of the EUT being tested.

## WAVEFORM VERIFICATION

Basic test standards require that the simulator output be verified periodically. In the case of the Pulse Magnetic Field, verification is accomplished by verifying the amplitude of the  $8/20\mu\text{s}$  current pulse driving the coil. An appropriate current transformer (Pearson Model 110 or equivalent) and an oscilloscope with a bandwidth of  $>100\text{MHz}$  capable of displaying a single pulse are required.

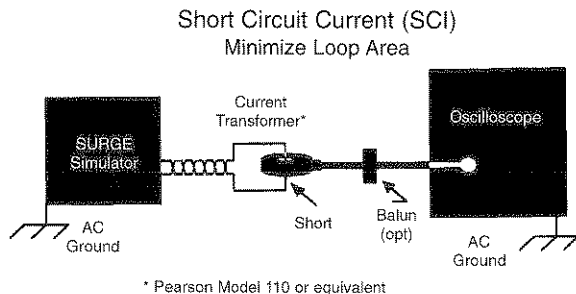

## TEST EXECUTION

According to IEC 1000-4-9, tests must be performed in compliance with the manufacturer's test plan, which shall specify:

- How the test is performed
- Verification of the laboratory reference conditions
- Preliminary verification of the correct operation of the EUT
- An evaluation of the test results

## TEST APPLICABILITY

According to Annex A of IEC 1000-4-9, test levels shall be selected in accordance with the most realistic installation and environmental conditions. Tests are recommended for equipment operating in areas characterized by proximity of conductors of lightning protection systems and or structures, or the proximity of conductors, bus-bars or medium to high voltage lines carrying tens of kA.

## PULSE MAGNETIC FIELD SIMULATORS

Pulse Magnetic Field Simulators and standard coils provided by KeyTek Instrument Corporation meet the pulse waveform and amplitude requirements for testing to  $>1000\text{A/m}$  in accordance with IEC 1000-4-9. Consult KeyTek for larger coils used for testing floor standing equipment. Contact KeyTek for details.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek is a registered trademark of Thermo Voltek Corporation. ©Thermo Voltek.  
Specifications are subject to change without notice. Printed in USA. 10/97

# PULSED EMI

Models CM-ESD and PRO-ESD ACCESSORIES

## Electrostatic Discharge



*ESD accessories for Electrostatic Discharge (ESD) testing beyond IEC 1000-4-2 with the CEMASTER® and EMCPro™ Compliance-Level Immunity Test Systems.*

### CM-ESD and PRO-ESD ACCESSORIES

---

#### Diagnostic E and H-Field Simulation

- **MZT-11** – E-Field Simulation Tip:  
Provides repeatable, local **static** E-Field simulation for interrogating high-impedance circuits for upsets due to various levels of fixed or slowly changing electric fields.

Provides repeatable, fast rise time, local **dynamic** E-Field simulation, while simultaneously minimizing the effects of local ESD-generated H-Fields. The purpose is to isolate circuits sensitive to real-world ESD E-Fields, which often have sub-nanosecond edges.

- **MZT-12** – H-Field Simulation Tip provides repeatable, local dynamic H-Field simulation, while simultaneously minimizing the magnitude of local ESD-generated E-Fields. Analogous with dynamic E-Field simulation, the purpose of diagnostic H-Field simulation is to isolate circuits sensitive to real-world ESD H-fields, which often have super-fast rise times.

#### Vertical & Horizontal Coupling Plane For Indirect ESD Testing

- **VCP-1** – Vertical Coupling Plane for indirect ESD tests per IEC 1000-4-2 is used to simulate the effects of human body ESD events to metal objects adjacent to an EUT. The specified 0.5 x 0.5m vertical coupling plane includes: insulation at back of plane for personal protection, convenient bench stand for hands-off testing, handles and camera tripod mount to facilitate off-bench use.
- **HCP-1** – Horizontal Coupling Plane for indirect ESD tests per IEC 1000-4-2 is used to simulate the effects of human body ESD events to a metal bench or desk on which the EUT may be resting. The specified 1.6 x 0.8m horizontal coupling plane includes a roll of <.5mm thick, static-dissipative sheet insulator for use above the plane for personal protection (meets IEC 1000-4-2 insulation thickness requirements).

# Models CM-ESD and PRO-ESD ACCESSORIES

---

## AIR DISCHARGE AND CONTACT MODE TESTING

---

- TPC-3:** Replacement contact mode tip for direct ESD tests in accordance with the rise times specified in IEC 1000-4-2 (0.7 - 1ns)
- TPA-2:** Replacement air discharge tip for ESD tests in accordance with IEC 1000-4-2

---

## CALIBRATION TESTING

---

- CTC-3:** Coaxial current monitor: IEC 1000-4-2 coax monitor for ESD current waveform, with 1GHz capability. Includes high-peak-power attenuator and low loss scope cable. IEC and ANSI require mounting the target in a 1.5m x 1.5m plane. See TP-3 accessory
- FCS-1:** Field and Corona Sensor Group: Common Monitor Unit HEC-1, H-Field sensor HFS-1, E-Field sensor EFS-1 and Pre-Discharge corona sensor CCS-1
- DCA-2:** DC Output Calibration Attenuator for an independent measurement of the ESD voltage on the tip of the CM-ESD
- 

---

## ADDITIONAL OPTIONS

---

- TP-3:** Full, 1.5m x 1.5m (59" x 59") IEC 1000-4-2 and ANSI C63.16 Target Plane, for mounting the CTC-3 coaxial target
- T-2:** A non-conducting tripod which holds the CM-ESD or PRO-ESD simulator steady against equipment being tested with hundreds of discharges at a single point, without interfering with the test results
- MCA-1:** Hard Carry Case (does not include space for VCP-1, HCP-1, T-2 or TP-3)

---

## MINIMUM SYSTEM REQUIREMENTS

---

- CEMASTER:** CM-BASE and CM-ESD with CM-SW or CM-FP
- EMCPRO:** PRO-BASE and PRO-ESD
- 

*For additional CEMASTER® and EMCPro™ literature, call, email or fax the KeyTek sales department.*



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
<http://www.keytek.com>

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and CEMASTER are registered trademarks and EMCPro and CEWare are trademarks of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.




# KeyTek EMC Immunity Test System

## SELECTOR GUIDE

Standards	Test Purpose & Description	MiniZap®	CEMASTER®	EMCPro™	ECAT®	G-STRIP™	XCELL™
IEC 1000-4-2 Electrostatic Discharge ✓	Requirements for simulating human ESD. Contact mode preferred for direct ESD; contact mode only for indirect ESD	15kV air 8.8kV contact	8.8kV air 4.4kV contact	8.8kV air 4.4kV contact	16kV air 8kV contact	*	*
IEC 1000-4-3	Radio frequency radiated immunity test (pre-compliance)	*	*	*	*	100kHz to 1GHz to 32V/m	*
IEC 1000-4-3	Radio frequency radiated immunity test (compliant)	*	*	*	*	*	26 MHz to 1GHz to 20V/m
IEC 1000-4-4 ✓ Electrical Fast Transients <i>LIGHTNING STRIKE</i>	Requirements for simulating "sanitized" showering arc, on both power and I/O (data and signal) lines	*	2.5kV	4.4kV	8kV	*	*
IEC 1000-4-5 ANSI C62.41 Surge 1.2/50µs, 8/20µs Combination Wave Category B	Requirements for simulating surges on both power and I/O (data and signal) lines	*	2.5kV	6kV	22kV	*	*
IEC 1000-4-5 Surge 10/700µs Telecom Wave	Requirements for simulating surges on telecommunication lines	*	*	6.6kV	7kV	*	*
IEC 1000-4-6	Radio frequency conducted immunity test (compliant)	*	*	*	*	IEC levels 1, 2 & 3 to 10V	*
IEC 1000-4-8 Frequency Magnetic	Magnetic fields generated by AC power mains	*	4A/m	4A/m	*	*	*
IEC 1000-4-9 Pulse Magnetic Fields	Simulates pulsed fields found in power stations, substations and other environments where very high transients occur	*	800A/m	1000A/m	> 1000A/m	*	*
IEC 1000-4-11 Dips and Interrupts	Simulates voltage fluctuations of the mains	*	70%, 40%,	70%, 40%, 0% short and open	150%, 120%, Dips 110%, 100%, 90%, 80%, 70%, 40%, 0% short and open	*	*
ANSI C62.41 Surge Ring Wave Category A, B	Requirements for simulating 100kHz ring wave	*	*	6.6kV	6.6kV	*	*
EN55011, EN55022, EN55014, FCC Part 15	Radio frequency radiated emissions testing (pre-compliance)	*	*	*	*	100kHz to 1GHz	26MHz to 1GHz
CCITT Rec. K.17, K.20, K.21 Surge 10/700µs Telecom Wave	For qualifying telecom repeaters, central office and station (i.e., subscriber) equipment	*	*	6.6kV	7kV	*	*
UL 1449 Surge Combination Waves	Qualification tests for AC powerline protectors. Three levels of 6kV combination wave required: 3kA, 750A and 500A	*	*	3kA	3kA, 750A, 500A	*	*
FCC Part 68 Telecom	For qualifying telecom equipment: specifies surge tests on telecom lines	*	*	*	10/160µs waveform, 1500V; 10/560µs waveform, 800V	*	*
FCC Part 68 Power Lines	For qualifying telecom equipment: specifies surge tests on power lines	*	*	*	2/10µs waveform, 2500V	*	*
GR-1089-CORE Core	Surge test requirements for telecom equipment installed in various locations	*	*	*	2/10µs waveform, 800V, 1500V, 5000V (AC mains)  10/360µs waveform 1000V  10/1000µs waveform 600V, 1000V, 1500V	*	*

\* Not applicable

# KeyTek Representatives & Distributors Worldwide

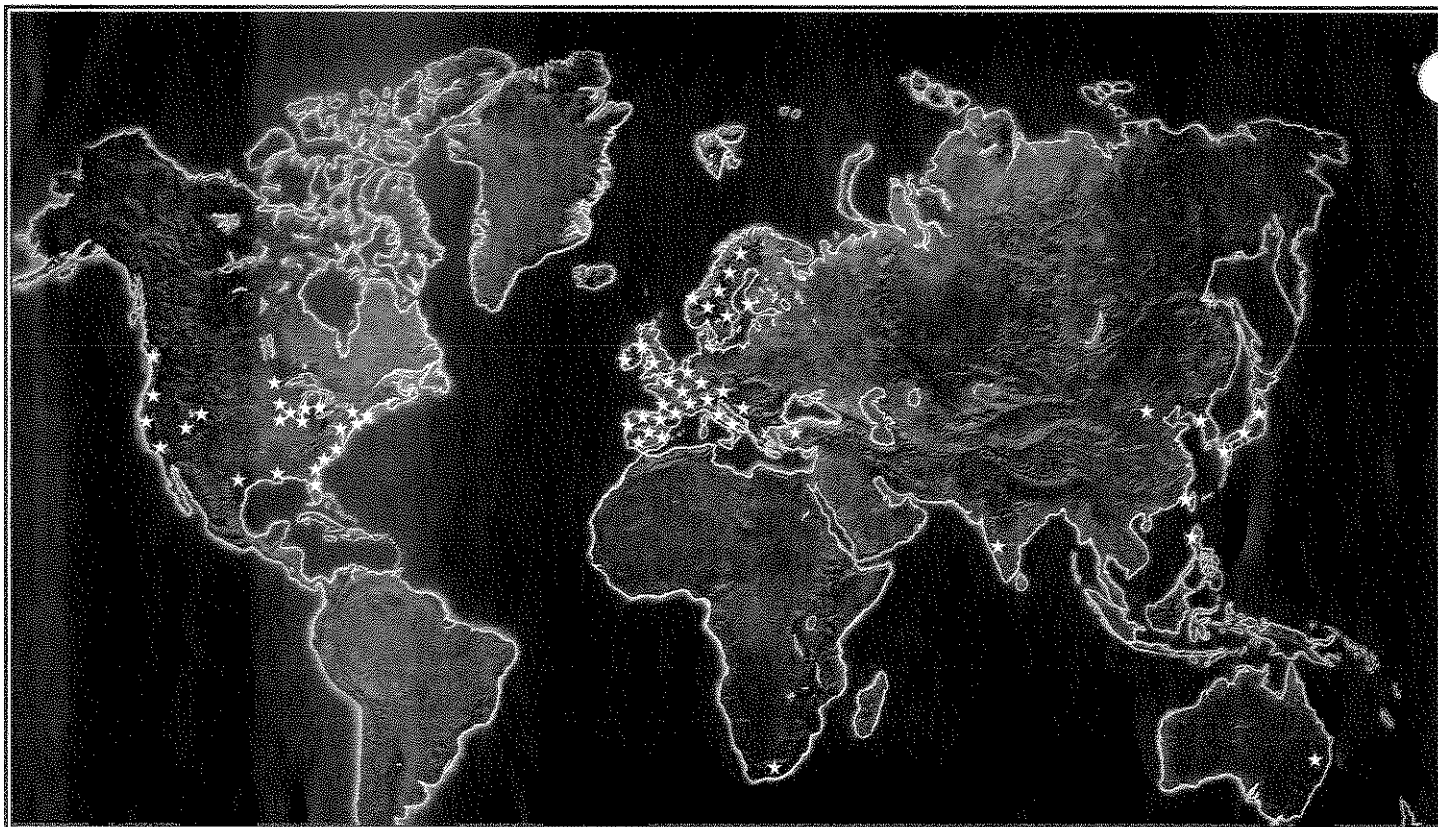

## NORTH AMERICA

NY	USA	Martin P. Andrews	315-637-5291
NY	USA	Bytec	516-781-7400
OH	USA	Micro Sales Corporation	614-792-9117
MO	USA	Dynamic Technology, Inc.	314-567-1984
VA	USA	Electronic Resources Inc.	540-289-5571
MN	USA	Hei-Lite/Murnco Sales	612-854-4161
AL	USA	Kemp Instruments, Inc.	205-837-4304
IL	USA	Loren Green Associates	847-550-1028
PA	USA	Robert Meyers Associates	215-635-1331
CO	USA	Sierra Technical Group	303-790-1700
AZ	USA	Sierra Technical Group	602-894-2335
NC	USA	Teqspec III Inc.	910-765-5553
CA	USA	Western Digital & Instrumentation	415-591-6535
FL	USA	TeqSpec-FLA	813-942-6006
CA	USA	Technologies West, Inc.	714-766-9495
TX	USA	J. Wisdom & Associates, Inc	972-470-9093
NH	USA	Starboard Sales	603-898-3284
OR	USA	Northwest Test & Measurement	503-645-9000
MI	USA	Consulting Engineers	616-445-2415
IL	USA	Transient Specialties	708-246-3297
ONT	Canada	MULTILEK Inc.	613-226-2365

## INTERNATIONAL

VIC	Australia	Scientific Devices Australia Pty Ltd.	61-3-9569-1366
	Britain	HF Instruments	44-1252-855500
	Denmark	Metric A/S	45-43-71-64-44
	Finland	Klinkmann	35-89-513322
	France	KMP	33-1-46-450945
	France	Opilas Systemes	33-16-0795920
	Germany	EMCO Elektronik (Pulsed EMI Products)	49-89-8562071
	Germany	env GmbH (RF Products)	49-89-6141 710
	Greece	Marac	30-1-431-4361
	Holland	Comtest Instrumentation B.V.	31-71-5-417531
	India	Microtek Instruments	91-44-4330024
	Ireland	Data Edge Ltd.	3531-284-9666
	Israel	Racom Electronics Co. Ltd.	972-3-577-6800
	Italy	Comtest Italia s.r.l. (EMC Products)	39-11-455-1388
	Italy	Elexind (Component Reliability Products)	39-2-921-03554
	Japan	Toyo Corporation	81-3-5688-6800
	Korea	keytek corporation	82-2501-4277
	Norway	Instrument OG Data Systemer A.S.	47 66 98 18 70
	Singapore	TME Systems PTE Ltd.	65-74-77-234
	Spain	Alava Ingenieros	34-1-572-0440
	Sweden	MTT AB	46 8 792 61 00
	Sweden	Technology Marketing	46-18-10 70 50
	Switzerland	Emitec AG	41-41-748-60-10
	Switzerland	Telemeter Electronic AG	41-71 699 20 20
	Taiwan	Kimpson	886-2-2916-0715
	Turkey	Norana	90-232-421-787




One Lowell Research Center  
 Lowell, Massachusetts 01852-4345 USA  
 1 800 753 9835 •  
 Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
 email: sales@keytek.com  
 http://www.keytek.com



# CEMASTER®

Model CM-HPWR

## Power Frequency Magnetic Field

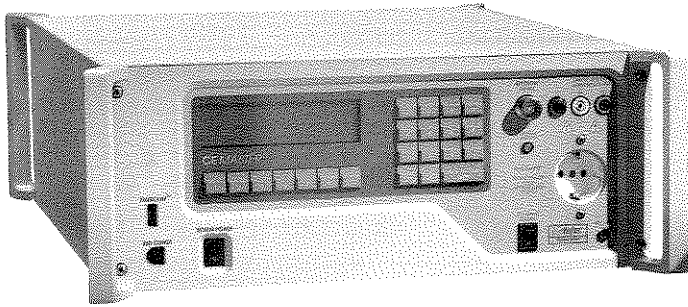

*Provides Power Frequency Magnetic Field test capability to IEC 1000-4-8 for the CEMASTER® Compliance-Level Immunity Tester.*

### FEATURES

---

- **Provides compliance-level** testing to meet the requirements of the EMC Directive and obtain the CE Mark.
- **Exceeds test levels** outlined in the Generic Immunity and Product Family Standards for power frequency magnetic fields.
- **Generates 50 or 60Hz fields** independent of input mains frequency.
- **Configurable** with any combination of 5 additional immunity test standards in a single tester.
- **Computer control** via software or front panel.
- **Predefined IEC test routines** from both software and front panel control.
- **Windows® 3.1 and 95 based** application software and/or front panel keypad and graphics display.
- **Optional** low cost coil (CM-HCOIL) is calibrated to the CEMASTER.

### SYSTEM BENEFITS

---

- **Batch IEC test sequences** significantly reduce test throughput times by running entire IEC test sequences in a single pass.
- **Pre-programmed IEC 1000-4-8 test routines** save time and decrease the potential for human error.
- **Automatic compliance report generation, using option CEWare™**, provides Power Frequency Magnetic Field test results in a format suitable for archiving CE Mark test records.
- **Light weight, ergonomic design** provides maximum flexibility for operating the CEMASTER from a table top, floor or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the tester between test departments or to remote facilities.

# Model CM-HPWR

## OUTPUT SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

<b>Field Frequency:</b>	50/60Hz
<b>Field Amplitude:</b>	0.5 to 4.0A/m in 0.25A steps, ±10% accuracy (with CM-HCOIL)
<b>Coil Factor:</b>	0.65 to 1.00 (Maximum output 4.0A/m with coil factor 0.8 linearly derated to 3.25A/m with coil factor 0.65)
<b>Coil Resistance:</b>	0.05Ω maximum
<b>AC Source:</b>	Internal to CEMASTER

### WAVEFORM VERIFICATION

Basic test standards require that the simulator output be verified periodically. For magnetic fields, it is only the amplitude that needs to be verified. This is accomplished with KeyTek's CM-HMON or other commercially available magnetic field probe and monitor.

### MINIMUM SYSTEM REQUIREMENTS

#### CM-BASE with CM-SW or CM-FP

### AVAILABLE OPTIONS

<b>CM-HCOIL:</b>	1m by 1m coil used to produce the magnetic fields
<b>CM-HMON:</b>	Magnetic field measurement instrument for verifying the amplitude of the magnetic fields produced by the CM-HPWR Module
<b>HPOWER-EXT:</b>	External generator for power frequency magnetic field to 30A/m

### AN AFFORDABLE EMC IMMUNITY TESTER THAT DOES IT ALL

The CEMASTER® is designed from the ground up to provide compliance-level testing to the standards manufacturers must meet in order to compete in today's international marketplace.

Each CEMASTER is custom configured to meet your specific needs and budget requirements. When completely configured, the CEMASTER provides compliance-level testing to IEC 1000-4-X Series Immunity Standards for:

- IEC 1000-4-2 ESD
- IEC 1000-4-4 EFT
- IEC 1000-4-5 Surge
- IEC 1000-4-8 Power Frequency Magnetic Field
- IEC 1000-4-9 Pulse Magnetic Field
- IEC 1000-4-11 Dips & Interrupts

## CEMASTER PLATFORM (CM-BASE)

### RATINGS AND POWER REQUIREMENTS

#### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7 ("Schuko") or BS 1363 (British Standard)

### POWER REQUIREMENTS

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

*For additional CEMASTER® literature, call, email or fax the KeyTek sales department.*



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and CEMASTER are registered trademarks and CEWare is a trademark of  
Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change  
without notice. Printed in USA.

# CEMASTER®

Model CM-ESD

## Electrostatic Discharge



*Provides Electrostatic Discharge (ESD) test capability to IEC 1000-4-2 for the CEMASTER Compliance-Level Immunity Tester.*

### FEATURES

- **Provides compliance-level testing** to meet the requirements of the EMC Directive and obtain the CE Mark.
- **LED voltage display** directly samples and indicates actual tip voltage.
- **Configurable** with any combination of 5 additional immunity test standards in a single tester.
- **Predefined IEC test routines** from both software and front panel control.
- **Windows® 3.1 and 95 based application software** and/or front panel keypad and graphics display.
- **Built-in shot counter and timer**
- **Premium storage case** for ESD simulator and accessories.
- **Portable**, light weight design for ease of use.

### SYSTEM BENEFITS

- **Batch IEC test sequences** significantly reduce test throughput times by running entire IEC test sequences in a single pass.
- **Pre-programmed IEC 1000-4-2 test routines** save time and decrease the potential for human error.
- **Automatic compliance report generation, using option CEWare™**, provides ESD test results in a format suitable for archiving CE Mark test records.
- **Built-in shot counter and timer** provides optimum control over the number of shots delivered to the EUT and time between test events.
- **Light weight, ergonomically designed CM-ESD** provides a comfortable, easy to use device capable of continuous testing.

# Model CM-ESD

## OUTPUT SPECIFICATIONS AND TOLERANCES


### CM-ESD

#### ELECTRICAL

<b>Peak Air Discharge:</b>	500V to 8.8kV; 1V resolution, ±5% accuracy
<b>Peak Contact Discharge:</b>	500V to 4.4kV; 1V resolution, ±5% accuracy
<b>Rise Time:</b>	0.7 to 1ns
<b>Repetition Rate:</b>	Single-shot, 1 pulse/second and 20 pulses/second
<b>Accessories:</b>	See ESD Accessory Sheet

#### WAVEFORM VERIFICATION

The basic test standards require that the simulator output be verified periodically. A Model CTC-3 measurement target and target plane is required for ESD current waveform verification. The ESD current measurement is then made using an oscilloscope having a 1GHz or greater bandwidth.

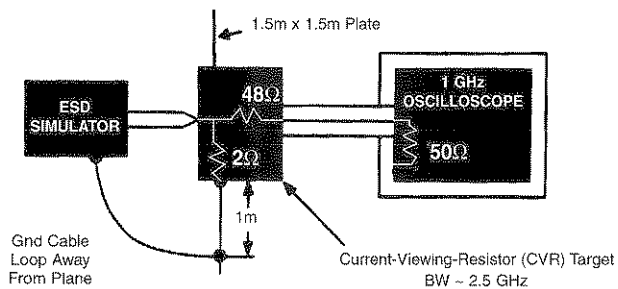

#### MINIMUM SYSTEM REQUIREMENTS

### CM-BASE with CM-SW or CM-FP

## AN AFFORDABLE EMC IMMUNITY TESTER THAT DOES IT ALL

The **CEMASTER**® is designed from the ground up to provide compliance-level testing to the standards manufacturers must meet in order to compete in today's international marketplace.

Each **CEMASTER** is custom configured to meet your specific needs and budget requirements. When completely configured, the **CEMASTER** provides compliance-level testing to IEC 1000-4-X Series Immunity Standards for:

- IEC 1000-4-2 ESD
- IEC 1000-4-4 EFT
- IEC 1000-4-5 Surge
- IEC 1000-4-8 Power Frequency Magnetic Field
- IEC 1000-4-9 Pulse Magnetic Field
- IEC 1000-4-11 Dips & Interrupts

## CEMASTER PLATFORM (CM-BASE)

#### RATINGS AND POWER REQUIREMENTS

#### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7 ("Schuko"), BS 1363 (British Standard)

#### Power Requirements

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

*For additional CEMASTER® literature, call, email or fax the KeyTek sales department.*




One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and **CEMASTER** are registered trademarks and **CEWare** is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.

# CEMASTER®

Model CM-HPULSE

## Pulse Magnetic Field

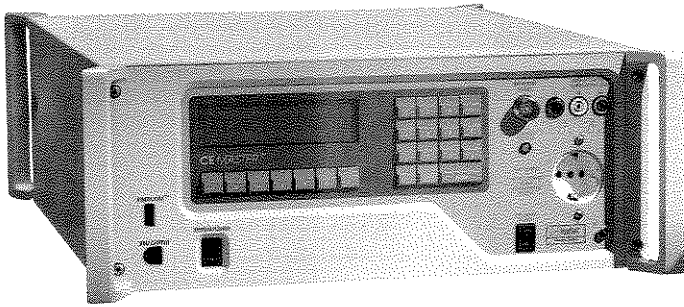

*Provides Pulse Magnetic Field test capability to IEC 1000-4-9 for the CEMASTER Compliance-Level Immunity Tester.*

### FEATURES

---

- **Provides compliance-level** testing to meet the requirements of the EMC Directive and obtain the CE Mark.
- **Exceeds test levels** outlined in the Generic Immunity and Product Family Standards for pulse magnetic fields.
- **Configurable** with any combination of 5 additional immunity test standards in a single tester.
- **Optional low cost coil** (CM-HCOIL) is fully calibrated to the CEMASTER
- **Predefined IEC test routines** from both software and front panel control.
- **Windows® 3.1 and 95 based** application software and/or front panel keypad and graphics display.

### SYSTEM BENEFITS

---

- **Batch IEC test sequences** significantly reduce test throughput times by running entire IEC test sequences in a single pass.
- **Pre-programmed IEC 1000-4-9 test routines** save time and decrease the potential for human error.
- **Automatic compliance report generation, using option CEWare™**, provides Pulse Magnetic Field test results in a format suitable for archiving CE Mark test records.
- **Light weight, ergonomic design** provides maximum flexibility for operating the CEMASTER from a table top, floor or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the tester between test departments or to remote facilities.

# Model CM-HPULSE

## OUTPUT SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

<b>Current Waveform:</b>	8/20 $\mu$ s
<b>Field Amplitude:</b>	50A/m to 800A/m <sup>1</sup> $\pm$ 10% accuracy ( <sup>1</sup> Based on coil factor of .72 or greater)

### WAVEFORM VERIFICATION

Basic test standards require that the simulator output be verified periodically. For the magnetic fields, verification is accomplished by verifying the amplitude of the 8/20 $\mu$ s current pulse driving the coil. An appropriate current transformer (Pearson Model 110 or equivalent) and an oscilloscope with a bandwidth of >100MHz capable of displaying a single pulse are required.

### MINIMUM SYSTEM REQUIREMENTS

#### CM-BASE with CM-SW or CM-FP, CM-SURGE

### AVAILABLE OPTIONS

<b>CM-HMON:</b>	Measurement probe for power frequency magnetic fields
<b>CM-HCOIL:</b>	1m by 1m coil used to produce the magnetic fields

## AN AFFORDABLE EMC IMMUNITY TESTER THAT DOES IT ALL

The **CEMASTER**<sup>®</sup> is designed from the ground up to provide compliance-level testing to the standards manufacturers must meet in order to compete in today's international marketplace.

Each **CEMASTER** is custom configured to meet your specific needs and budget requirements. When completely configured, the **CEMASTER** provides compliance-level testing to IEC 1000-4-X Series Immunity Standards for:

- IEC 1000-4-2 ESD
- IEC 1000-4-4 EFT
- IEC 1000-4-5 Surge
- IEC 1000-4-8 Power Frequency Magnetic Field
- IEC 1000-4-9 Pulse Magnetic Field
- IEC 1000-4-11 Dips & Interrupts

## CEMASTER PLATFORM (CM-BASE)

### RATINGS AND POWER REQUIREMENTS

#### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V rms
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7 ("Schuko"), or BS 1363 (British Standard)

### POWER REQUIREMENTS

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

*For additional CEMASTER<sup>®</sup> literature, call, email or fax the KeyTek sales department.*



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com


A division of Thermo Voltek, a Thermo Electron company  
KeyTek and CEMASTER are registered trademarks and CEWare is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.



# CEMASTER®

**Model CM-PQF**

## Dips & Interrupts

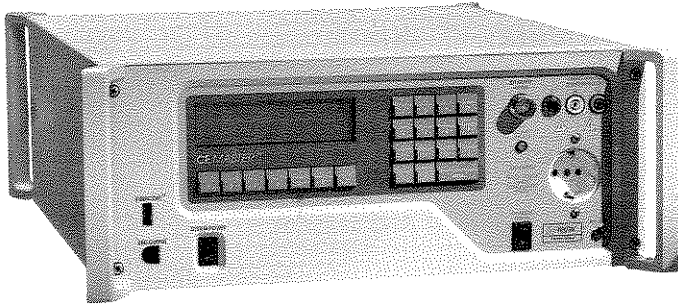

*Provides Dips and Interrupts test capability to IEC 1000-4-11 for the CEMASTER® Compliance-Level Immunity Tester.*

### FEATURES

---

- **Provides compliance-level testing** to meet the requirements of the EMC Directive and obtain the CE Mark.
- **Meets all test levels** outlined in the Generic Immunity and Product Family Standards for dip and interrupt testing.
- **Configurable** with any combination of up to 5 immunity standards in a single tester.
- **Includes built-in transformer** for fast, reliable operation. No external hardware required.
- **Built-in, high-speed tap switching** allows custom test routines where high speed switching between levels is required - not just to 100%.
- **Predefined IEC test routines** controlled from either software or front panel.
- **Windows® 3.1 and 95 based application software** and/or front panel keypad and graphics display.

### SYSTEM BENEFITS

---

- **Batch IEC test sequences** significantly reduce test throughput times by running entire IEC test sequences in a single pass.
- **Pre-programmed IEC 1000-4-11 test routines** save programming time and decrease the potential for human error.
- **Automatic compliance report generation, using option CEWare™**, provides Dips and Interrupts test results in a format suitable for archiving CE Mark test records.
- **Light weight, ergonomic design** provides maximum flexibility for operating the CEMASTER from a table top, floor or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the tester between test departments or to remote facilities.

# Model CM-PQF


## OUTPUT SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

<b>Dips:</b>	To 70% and 40% of nominal
<b>Interrupts:</b>	0% short or open
<b>Transition Time:</b>	1 $\mu$ s to 5 $\mu$ s into 100 $\Omega$
<b>Inrush Current:</b>	>250A at 120V; >500A at 240V
<b>Minimum Event:</b>	10°, 460 - 555 $\mu$ sec (based on 50/60 cycles)
<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous

### WAVEFORM VERIFICATION

The basic test standards require that the simulator output be verified periodically. For Dip & Interrupt test simulators, it is necessary to verify the voltage levels, transition times, and the inrush current capability. Most modern oscilloscopes are capable of observing the voltage levels and transition times. For verifying the inrush current, a bridge rectifier, suitably rated 1700 $\mu$ F capacitor, and appropriate current transformer are required, Model PQF-QUAL.

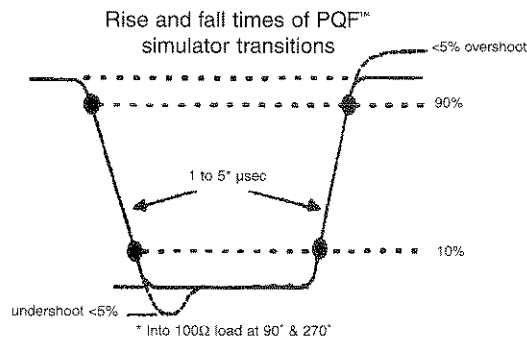

## AN AFFORDABLE EMC IMMUNITY TESTER THAT DOES IT ALL

The **CEMASTER**® is designed from the ground up to provide compliance-level testing to the standards manufacturers must meet in order to compete in today's international marketplace.

Each **CEMASTER** is custom configured to meet your specific needs and budget requirements. When completely configured, the **CEMASTER** provides compliance-level testing to IEC 1000-4-X Series Immunity Standards for:

- IEC 1000-4-2 ESD
- IEC 1000-4-4 EFT
- IEC 1000-4-5 Surge
- IEC 1000-4-8 Power Frequency Magnetic Field
- IEC 1000-4-9 Pulse Magnetic Field
- IEC 1000-4-11 Dips & Interrupts

### MINIMUM SYSTEM REQUIREMENTS

#### CM-BASE with CM-SW or CM-FP

### AVAILABLE OPTIONS

<b>CM-3PQF:</b>	16 Amp, 3-phase Dip/Interrupt selector.
<b>PQF-QUAL:</b>	External circuit per IEC 1000-4-11 for testing any PQF generator's inrush capability.

### CEMASTER PLATFORM (CM-BASE)

#### RATINGS AND POWER REQUIREMENTS

##### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7("Schuko"), or BS 1363 (British Standard)

#### POWER REQUIREMENTS

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

For additional **CEMASTER**® literature, call, email or fax the KeyTek sales department.




One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and **CEMASTER** are registered trademarks and **CEWare** and **PQF** are trademarks of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.

# PULSED EMI

Models CM-3CD-16 and CM-3CD-32

## Combined EFT and Surge Mains Coupler/Decouplers

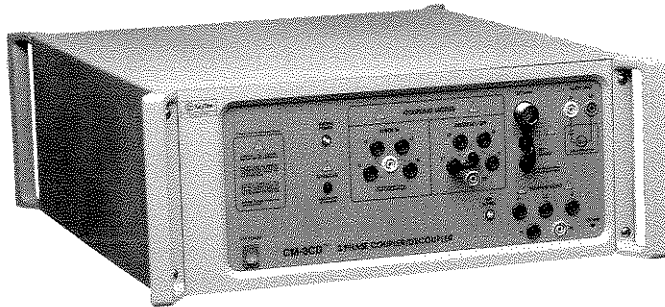

*Semi-automatic, three-phase AC/DC mains coupler/decouplers for EFT and Surge as specified by IEC 1000-4-4 and IEC 1000-4-5.*

### FEATURES

---

- AC voltages to 433V rms, DC to 100V.
- Continuous AC line currents to 32A/phase.
- Compatible with KeyTek's CEMASTER® and EMCPro™ for Surge and EFT, or any EFT simulator with user supplied cables.
- Low cost, standalone design.
- Comprehensive front panel design for easy mode selection.

### SYSTEM BENEFITS

---

- **Semi-automatic operation** when used with KeyTek's CEMASTER or EMCPro simulators reduces the possibility of test sequence errors by prompting the user to make coupling mode selections.
- **Pre-programmed IEC test routines** save time and decrease the potential for human error.
- **Automatic compliance report generation**, using option CEWare™, provides three-phase AC/DC line coupler/decoupler test results in a format suitable for archiving CE Mark test records.
- **Ergonomic design** provides maximum flexibility for operating from a table top or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the unit between departments or remote facilities.

# Models CM-3CD-16 and CM-3CD-32

## SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

#### Waveforms:

**EFT:** 5/50ns, per IEC 1000-4-4  
**Surge:** Combination wave:  
1.2/50 $\mu$ s open-circuit voltage,  
8/20 $\mu$ s short-circuit current,  
per IEC 1000-4-5

#### Maximum Surge

**Voltage & Current:** 6.6kV, 3.3kA

#### Maximum EFT

**Voltage:** 4.4kV

#### Coupling Modes:

**EFT:** L1, L2, L3, N or PE  
**Surge Hi:** L1, L2, L3 or N  
**Surge Lo:** L1, L2, L3, N or PE

### COUPLER/DECOUPLERS

**AC Voltage:** 50 to 250V, 50/60Hz line to ground, 50 to 433V line to line

#### AC Current:

**CM-3CD-16** 16A/phase continuous  
**CM-3CD-32** 32A/phase continuous

#### DC Current:

**CM-3CD-16:** 16A up to 48V  
8A up to 110V  
1.2A up to 220V  
0.3A up to 440V  
**CM-3CD-32:** 25A up to 48V  
8A up to 220V  
1.2A up to 220V  
0.3A up to 440V

#### EUT Mains Output

**Connectors:** Safety Sockets

### POWER REQUIREMENTS

**Input Voltage:** 90-250VAC, 50/60Hz

**Input Current:** 1A at 120VAC; 0.5A at 240VAC

### PHYSICAL

**Height:** 18cm (7")  
**Width:** 47cm (18.5")  
**Depth:** 56cm (22")  
**Weight:**  
**CM-3CD-16** 17kg (38 lbs)  
**CM-3CD-32** 24kg (52 lbs)

### MINIMUM SYSTEM REQUIREMENTS

**CEMASTER, EMCPro** or any simulator with EFT test capability

*For additional Pulsed EMI literature, call, email or fax the KeyTek sales department.*




One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
<http://www.keytek.com>

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and CEMASTER are registered trademarks and EMCPro and CEWare are trademarks of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.

# PULSED EMI

Model CM-TELCD

## Telecom Line Coupler/Decoupler

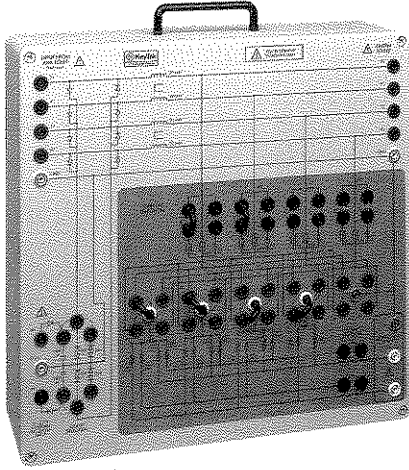

*Provides the ability to couple both the telecom wave and combination wave per IEC 1000-4-5.*

### FEATURES

---

- **Fully compliant** with IEC 1000-4-5 requirements for telecom line coupler/decouplers.
- **Permits compliance level testing** of telecom lines to Generic Immunity and Product Family Standards.
- **Built-in user selectable clamping circuit** provides additional protection for sensitive and costly auxiliary equipment.
- **Built-in multiple coupling devices**, including resistors for both 1.2/50 $\mu$ s and 10/700 $\mu$ s generators, 90V & 300V gas arresters and 0.1 $\mu$ F capacitors.
- **Symmetric coupling** per IEC 1000-4-5 for telecommunication lines.
- **Data rates to greater than 100kHz**
- **Comprehensive front panel wiring aids.**

### SYSTEM BENEFITS

---

- **Semi-automatic operation when used with KeyTek simulators** reduces the possibility of test sequence errors by prompting the user to make the correct selections.
- **Portable architecture** enables users to easily transport the unit between test departments or remote facilities.
- **Standard CM-TELCD design** ensures high speed transmission.
- **Air core decoupling chokes** allow use of DC signals without problems due to core saturation.

# Model CM-TELCD

## SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

<b>Waveforms:</b>	Designed to couple 1.2/50 $\mu$ s combination or 10/700 $\mu$ s telecom waves.
<b>Telecom Line Frequency:</b>	To 100kHz without significant degradation
<b>Number of Lines:</b>	Up to four lines - one or two pairs of balanced Telecom lines
<b>Maximum Surge Voltage:</b>	4.4kV
<b>Maximum Signal Line Voltage:</b>	200V
<b>Maximum Signal Line Current:</b>	1A AC or DC
<b>Clamping:</b>	Selectable built-in clamps of 20V and 225V: external bias input for other clamp levels

### PHYSICAL

<b>Height:</b>	12.2cm (4.8")
<b>Width:</b>	40.1cm (15.8")
<b>Depth:</b>	40.4cm (15.9")
<b>Weight:</b>	53.9kg (24.5 lbs.)

### MINIMUM SYSTEM REQUIREMENTS

**EMCPro with PRO-SURGE, PRO-TELECOM or with any IEC 1000-4-5 or CCITT Rec. K.17 10/700 $\mu$ s waveform simulator**

*For additional Pulsed EMI literature, call, email or fax the KeyTek sales department.*




One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
<http://www.keytek.com>

A division of Thermo Volttek, a Thermo Electron company  
KeyTek is a registered trademark and EMCPro is a trademark of Thermo Volttek Corporation. ©Thermo Volttek. Specifications are subject to change without notice.  
Printed in USA.

# CEMASTER®

Model CM-BASE

## Platform

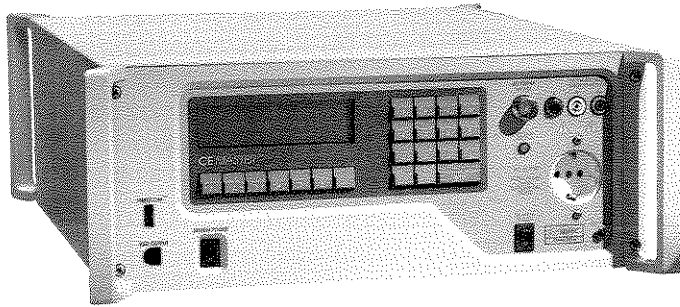

*A customer configured Immunity Tester for compliance testing to:*

*IEC 1000-4-2 ESD*

*IEC 1000-4-4 EFT*

*IEC 1000-4-5 Surge*

*IEC 1000-4-8 Power Frequency  
Magnetic Field*

*IEC 1000-4-9 Pulse Magnetic Field*


*IEC 1000-4-11 Dips & Interrupts.*

## FEATURES

- **A cost-effective, compliance-level** tester to be used as a primary test station, or to augment other test capabilities and stations in large facilities.
- **Customer configurable** Immunity Tester provides from one to six immunity tests in a single unit.
- **Windows® 3.1** and 95 based application software and/or front panel keypad and graphics display.
- **Pre-programmed IEC test routines** from both software and front panel control.
- **Portable**, light weight design.
- **Optional** transport case.
- **Optional** 19" rack mount kit.

## SYSTEM BENEFITS

- **Low cost, multi-standard** test system provides manufacturers with a single, stand-alone system solution.
- **Light weight, ergonomic design** provides maximum flexibility for operating the CEMASTER from a table top or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the tester between test departments or remote facilities.
- **Automatic compliance report generation**, using option CEWare™, provides test results in a format suitable for archiving CE Mark test records.

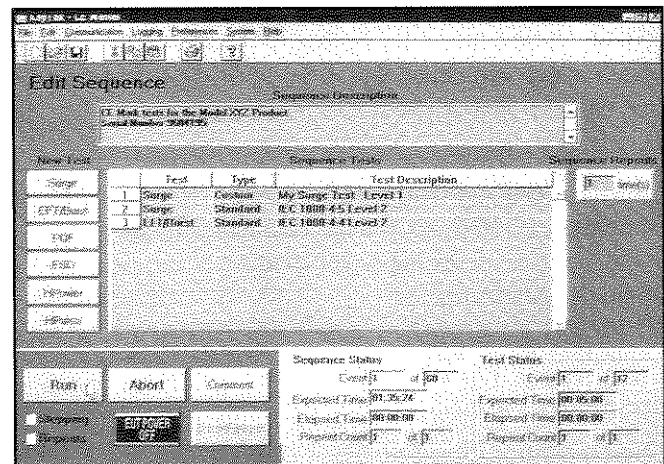

*Typical Software Screen Operating under Windows®*

# Model CM-BASE

## SPECIFICATIONS AND TOLERANCES

### CEMASTER IMMUNITY TEST LEVELS

<b>IEC 1000-4-2</b>	500V - 8.8kV Air Discharge 500V - 4.4kV Contact Mode
<b>IEC 1000-4-4</b>	250V - 2.5kV; 1- 100kHz
<b>IEC 1000-4-5</b>	250V - 2.5kV; 125A - 1.25kA
<b>IEC 1000-4-8</b>	0.5 - 4A/m AC H-Field
<b>IEC 1000-4-9</b>	50 - 800A/m Pulse Field
<b>IEC 1000-4-11</b>	100, 70, 40 and 0% short or open; inrush >250A @ 120V, and >500A @ 240V

### RATINGS AND POWER REQUIREMENTS

#### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7 ("Schuko"), or BS 1363 (British Standard)

### POWER REQUIREMENTS

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

### PHYSICAL

<b>Height:</b>	17.8cm (7")
<b>Width:</b>	47cm (18.5")
<b>Depth:</b>	56cm (22")
<b>Weight:</b>	29kg (64 lbs.)

### ENVIRONMENTAL

#### Operating Limits

<b>Temperature:</b>	15 - 40°C
<b>Humidity:</b>	10 - 75%, non-condensing
<b>Altitude:</b>	8000 feet max.

#### Storage Limits

<b>Temperature:</b>	0 - 60°C
<b>Humidity:</b>	10 - 90%, non-condensing
<b>Altitude:</b>	8000 feet max.

### MINIMUM SYSTEM REQUIREMENTS

**CM-BASE with CM-SW or  
CM-FP and at least one immunity test capability**

## AVAILABLE OPTIONS

### IMMUNITY TEST CAPABILITIES

<b>CM-ESD:</b>	Electrostatic Discharge (IEC 1000-4-2)
<b>CM-EFT:</b>	Electrical Fast Transient (IEC 1000-4-4)
<b>CM-SURGE:</b>	Surge (IEC 1000-4-5)
<b>CM-HPWR:</b>	Power Frequency Magnetic Field (IEC 1000-4-8)
<b>CM-HPULSE:</b>	Pulse Magnetic Field (IEC 1000-4-9)
<b>CM-PQF:</b>	Dips and Interrupts (IEC 1000-4-11)

### CONTROL FUNCTIONS

<b>CM-SW:</b>	Windows® based application software (CEWare™) provides the ability to run any sequence of predefined IEC routines or user defined immunity tests. User must purchase either CM-SW, CM-FP or both.
<b>CM-FP:</b>	Front Panel keypad and graphics display for manual operation or automatic control using predefined IEC routines. User must purchase either CM-SW, CM-FP or both.
<b>CM-SW/FP:</b>	Combines both software (CM-SW) and front panel (CM-FP) control functions.

### OTHER

<b>CM-RMK:</b>	19" Rack Mount Kit
<b>CM-CASE:</b>	Transportation case for the CEMASTER and accessories

*For additional CEMASTER® literature, call, email or  
fax the KeyTek sales department.*



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com


A division of Thermo Voltek, a Thermo Electron company  
KeyTek and CEMASTER are registered trademarks and CEWare is a trademark of  
Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change  
without notice. Printed in USA.



# CEMASTER®

**Model CM-EFT**

## Electrical Fast Transient

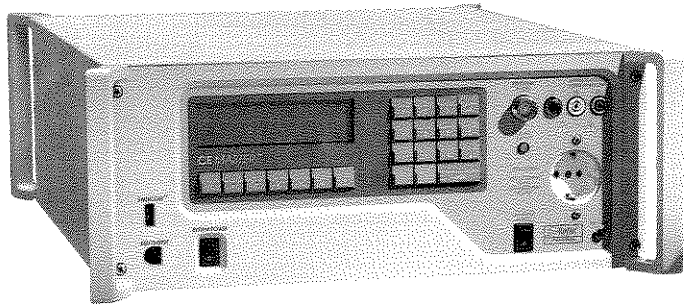

*Provides Electrical Fast Transient (EFT) test capability to IEC 1000-4-4 for the CEMASTER Compliance-Level Immunity Tester.*

### FEATURES

---

- **Provides compliance-level testing** to meet the requirements of the EMC Directive and obtain the CE Mark.
- **Exceeds the maximum test levels** outlined in the Generic Immunity and Product Family Standards.
- **Configurable** with any combination of 5 additional immunity test standards in a single tester.
- **Includes built-in** single phase mains coupler/decoupler for EUT's to 16A AC and to 10A DC.
- **Predefined IEC test routines** from both software and front panel control.
- **Windows® 3.1 and 95 based** application software and/or front panel keypad and graphics display.

### SYSTEM BENEFITS

---

- **Batch IEC test sequences** significantly reduce test throughput times by running entire IEC test sequences in a single pass.
- **Pre-programmed IEC 1000-4-4 test routines** save time and decrease the potential for human error.
- **Automatic compliance report generation, using option CEWare™**, provides EFT test results in a format suitable for archiving CE Mark test records.
- **Light weight, ergonomic design** provides maximum flexibility for operating the CEMASTER from a table top, floor or within a 19-inch rack.
- **Portable architecture** with rugged handles and optional transit case enables users to transport the tester between test departments or to remote facilities.

# Model CM-EFT

## OUTPUT SPECIFICATIONS AND TOLERANCES

### ELECTRICAL

<b>Peak Voltage:</b>	250V to 2.5kV; 1V resolution, ±10% accuracy
<b>Waveform:</b>	5ns/50ns impulse per IEC 1000-4-4
<b>Burst Period:</b>	300ms
<b>Burst Duration:</b>	15ms@ 1-5kHz, 0.75ms @ > 5kHz
<b>Frequency:</b>	1 - 100kHz in .5kHz steps, ±10% accuracy

### WAVEFORM VERIFICATION

The basic test standards require that the simulator output be verified periodically. For EFT, a high voltage 50 ohm load is required, and the measurement must be made using an oscilloscope with at least 400MHz bandwidth.

### MINIMUM SYSTEM REQUIREMENTS

**CM-BASE with CM-SW or CM-FP**

## AN AFFORDABLE EMC IMMUNITY TESTER THAT DOES IT ALL

The **CEMASTER**® is designed from the ground up to provide compliance-level testing to the standards manufacturers must meet in order to compete in today's international marketplace.


Each **CEMASTER** is custom configured to meet your specific needs and budget requirements. When completely configured, the **CEMASTER** provides compliance-level testing to IEC 1000-4-X Series Immunity Standards for:

- IEC 1000-4-2 ESD ✓
- IEC 1000-4-4 EFT
- IEC 1000-4-5 Surge
- IEC 1000-4-8 Power Frequency Magnetic Field ✓
- IEC 1000-4-9 Pulse Magnetic Field ✓
- IEC 1000-4-11 Dips & Interruptions ✓

*Pub. 1.1.01 EFT*

## AVAILABLE OPTIONS

- CM-3CD-16/32:** 16 or 32 Amp, 3-phase EFT and Surge coupler/decoupler
- CM-CCL:** Capacitive Coupling Clamp for coupling EFT transients to data lines in accordance with IEC 1000-4-4.

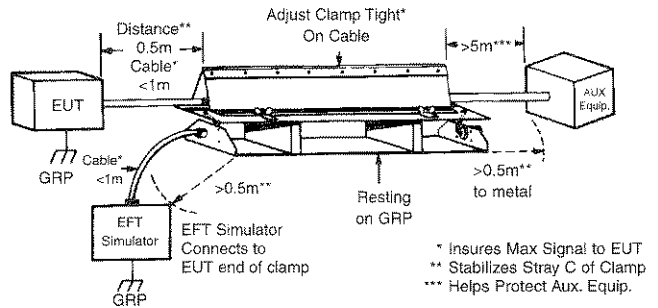

**CM-CCLC:** Interlocked Capacitive Coupling Clamp Cover and cables to be used with Model CM-CCL for increased safety.

**EFT-ATTN:** External EFT attenuator for oscilloscope monitoring of EFT pulses up to 4.4kV, 50 and 2K ohm input impedances. (Requires CM-EFT capability).

## CEMASTER PLATFORM (CM-BASE)

### RATINGS AND POWER REQUIREMENTS

#### Coupler/Decoupler

<b>AC Voltage:</b>	50 to 250V, 50/60Hz
<b>AC Current:</b>	16A continuous
<b>DC Voltage:</b>	0 to 100V
<b>DC Current:</b>	10A continuous
<b>EUT Connectors:</b>	NEMA 5-15, CEE7 ("Schuko") or BS 1363 (British Standard)

#### Power Requirements

<b>Input Voltage:</b>	90-250VAC, 50/60Hz
<b>Input Current:</b>	1A at 120VAC; 0.5A at 240VAC

For additional **CEMASTER**® literature, call, email or fax the KeyTek sales department.



One Lowell Research Center  
Lowell, Massachusetts 01852-4345 USA  
1 800 753 9835 • Tel: 1 978 275 0800 • Fax: 1 978 275 0850  
email: sales@keytek.com  
http://www.keytek.com

A division of Thermo Voltek, a Thermo Electron company  
KeyTek and **CEMASTER** are registered trademarks and **CEWare** is a trademark of Thermo Voltek Corporation. ©Thermo Voltek. Specifications are subject to change without notice. Printed in USA.

KPS-107B-11/97



